


# Analytical Methods

Accepted Manuscript

This article can be cited before page numbers have been issued, to do this please use: O. O. Fashedemi, O. C. Ozoemena, S. Peteni, A. B. Haruna, L. J. J. Shai, A. Chen, F. J. Rawson, M. Cruickshank, D. M. Grant, O. Ola and K. I. Ozoemena, *Anal. Methods*, 2025, DOI: 10.1039/D4AY01921K.

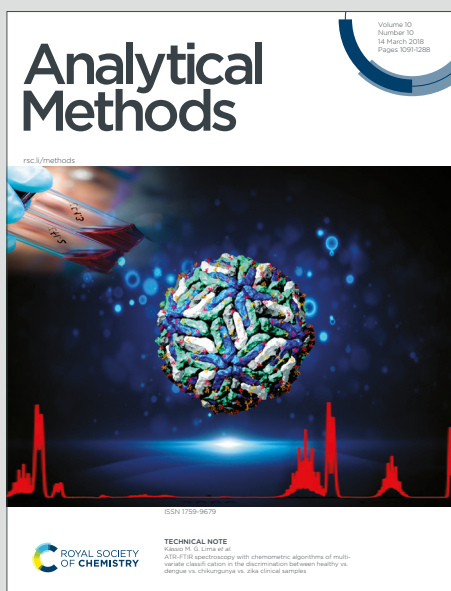

This is an Accepted Manuscript, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this Accepted Manuscript with the edited and formatted Advance Article as soon as it is available.

You can find more information about Accepted Manuscripts in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this Accepted Manuscript or any consequences arising from the use of any information it contains.

# Advances in Human Papillomavirus Detection for Cervical Cancer Screening and Diagnosis: Challenges of Conventional Methods and Opportunities for Emergent Tools

O. Fashedemi,<sup>a</sup> Okoroike C. Ozoemena,<sup>b</sup> Siwaphiwe Peteni,<sup>c</sup> Aderemi B. Haruna,<sup>c</sup> Leshweni J. Shai,<sup>d</sup> Aicheng Chen,<sup>b</sup> Frankie Rawson,<sup>a</sup> Maggie E Cruickshank,<sup>e</sup> David Grant,<sup>a</sup> Oluwafunmilola Ola,<sup>\*a</sup> and Kenneth I. Ozoemena<sup>\*c</sup>

Received 00th January 20xx,  
Accepted 00th January 20xx

DOI: 10.1039/x0xx00000x

Human papillomavirus (HPV) infection is the main cause of cervical cancer and other cancers such as anogenital and oropharyngeal cancers. The prevention screening and treatment of cervical cancer has remained one of the top priorities of the World Health Organization (WHO). In 2020, the WHO came up with the 90-70-90 strategy aimed at eliminating cervical cancers as a public health problem by the year 2030. One of the key priorities of this strategy is the recommendation for countries to ensure that 70% of their women are screened using a high-performance test by the age of 35, and again by the age of 45. Over the years, several traditional methods (notably, Pap smear and nucleic acid-based techniques) have been used for the detection of cervical cancer. While these methods have significantly reduced the incidence of cervical cancer and death, they still come short of excellence for the total eradication of HPV infection. The challenges include low sensitivity, low specificity, poor reproducibility, the need for high-level specialists, and the high cost of access to the facilities, to mention a few. Interestingly, however, several efforts are being made today to mitigate these challenges. In this review, we discussed the pros and cons of the traditional screening and testing of HPV infections, the efforts being made to improve their performances, and the emergent tools (especially, the electrochemical methods) that promise to revolutionize the screening and testing of HPV infections. The main aim of the review is to provide some novel clues to researchers that would allow for the development of high-performance, affordable, and triage-suitable electrochemical-based diagnostic tools for HPV and cervical cancer.

## Introduction

Persistent human papillomavirus (HPV) infection is the leading cause of cervical cancer. Cervical cancer remains the fourth most common cancer in women (after breast cancer, colorectal cancer, and lung cancer). According to the 2018 Report,<sup>1</sup> there were about 570 000 cases and 311 000 deaths arising from cervical cancer, mostly occurring in resource-limited countries in Sub-Saharan Africa, Asia, and Latin America. In sub-Saharan Africa, cervical cancer is the leading cause of cancer-related deaths in women. For example, Eswatini was reported as the country with the highest incidence, with about 6.5% of women developing cervical cancer before the age of 75 years. As part of the strategies to curb the incidence of cervical cancer and death, in August 2020 the WHO adopted the so-called 90-70-90 target for 2030: (i) 90% of girls to be fully vaccinated with the HPV vaccine by the age of 15, (ii) 70% of women screened using a high-

performance test by the age of 35, and again by the age of 45, and (iii) 90% of women with pre-cancer treated and 90% of women with invasive cancer managed.

All HPV genomic structure consists of a circular, double stranded DNA. Nearly all HPV have three distinct regions i.e. the long control region (LCR) or “L-region” which does not code for any proteins, the early region also known as the “E-region”, this encodes 6 viral proteins (E1, E2, E4, E5, E6, E7), E6 and E7 encodes two viral proteins which are oncogenic and lastly the late region (L-region), the L-region encodes structural proteins, L1 which is the major capsid protein and L2 the minor capsid protein. These proteins participate in the genomic replication, transcription, cell cycle, cell signalling and apoptosis control, immune modulation and structural modification of HPV infected cells.<sup>2,3</sup> Of the 14 high-risk HPV types, two of them (HPV-16 and HPV-18) are considered the most important as they have been observed in 62% of cervical cancers. Some literature states that HPV-16 and HPV-18 are responsible for up to 70% of cervical cancer cases, with HPV-16 present in about 60% of cases and HPV-18 in about 10%. HR-HPV encode specific viral genes, such as E6 and E7, which have been associated with cervical cancer cell lines. These viral genes produce oncoproteins that can be integrated into the hosts genome, such as E6 and E7 proteins. The E7 protein binds to

<sup>a</sup> Advanced Materials Group, Faculty of Engineering, The University of Nottingham, Nottingham NG7 2RD, U.K

<sup>b</sup> Department of Chemistry, University of Guelph, Ontario, Canada

<sup>c</sup> Molecular Science Institute, School of Chemistry, University of the Witwatersrand, Johannesburg 2050, South Africa

<sup>d</sup> Department of Biomedical Sciences, Tshwane University of Technology, Pretoria 0001, South Africa


<sup>e</sup> Aberdeen Centre for Women's Health Research, University of Aberdeen, Aberdeen AB25 2ZD, UK

† Footnotes relating to the title and/or authors should appear here.

Supplementary Information available: [details of any supplementary information available should be included here]. See DOI: 10.1039/x0xx00000x



## ARTICLE

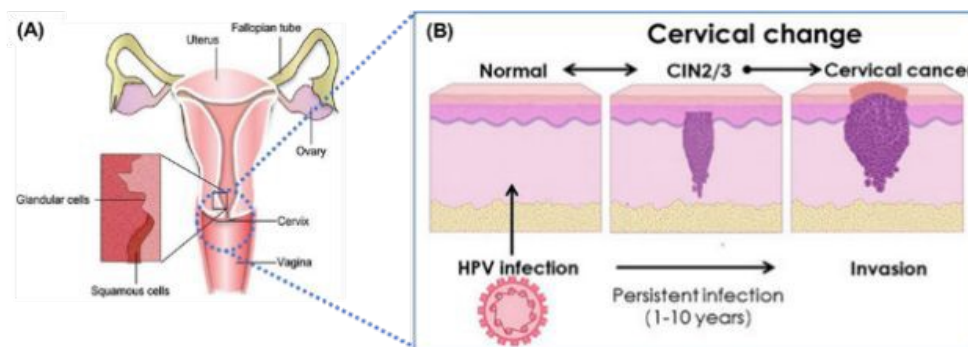View Article Online  
DOI: 10.1039/D4AY01921K

**Figure 1.** (A) Pictorial depiction of the cervix anatomy<sup>5</sup> (B) Schematic illustration of the cervical changes caused by HPV infection.<sup>6</sup>

retinoblastoma family proteins, impeding the inhibition of transcription factors and leading to uncontrolled cell cycle progression. Consequently, E7 protein degrades pRB function leading to an overexpression and disruption of the epithelial cell cycle, therefore leading to uncontrollable growth of cancerous cells.<sup>4</sup> HPV infection persistence can result in precancerous changes known as cervical intraepithelial neoplasia (CIN) which is curable if detected by screening when dysplastic cells are confined within the surface epithelium of the cervix. Cervical intraepithelial neoplasia (CIN) is in three stages: CIN1, CIN2, or CIN3. If left untreated, CIN2 or CIN3 (collectively referred to as CIN2+) can progress to cervical cancer as schematically shown in Figure 1. These have the potential to penetrate the basement membrane to become invasive cervical cancer and spread in nearby organs e.g., the uterus, bladder, rectum, and pelvic lymph nodes, thereby causing death. Apart from cervical cancer, hr-HPV are the causative agent of other cancers such as the anal, vulvar, penile, head and neck cancer.<sup>9-12</sup> Thus, early detection with low-cost and sensitive diagnostic devices will greatly benefit low-income areas. Precise and time-efficient measures could improve early diagnosis and treatment.

In Europe, cervical cancer remains the second most common cause of death in women aged between 15-44 years with reported diagnoses and death totalling 61,072 and 25,829, respectively. The incidence and mortality rates were estimated at 15.9 and 6.7 per 100 000 women in Europe, respectively, in comparison with a mortality rate of 6.8 per 100 000 women globally.<sup>13</sup> In the UK, the highest incidence rates were observed in young women between the ages 25-29 years.<sup>14</sup> Vaccination and screening have the potential to reduce the incidence rate of cervical cancer to 4 per 100 000 women globally.<sup>13</sup> Currently, there are 6 types of HPV vaccines that are approved by the FDA, namely 2vHPV (bivalent vaccine), 4vHPV (quadrivalent vaccine), and 9vHPV (9-valent vaccine), of the bivalent type, there are 2 vaccines and of the quadrivalent type, there are 3 vaccines. As their names suggest, the bivalent HPV vaccine can only be used for HPV 16 and 18, the quadrivalent can only be utilised for HPV 6, 11, 16 and 18, while the 9-valent HPV vaccine can be used for HPV 6, 11, 16, 18, 31, 33, 45, 52, and 58. Although the HPV vaccination programmes are meant to curb and control the progression of high-risk HPV to cervical cancer cases, LMICs are still burdened with poor vaccination rollouts, this can be contributed to a number of factors such as high cost of vaccine acquisition, lack of storage infrastructure

for vaccines, logistics etc. This, therefore, necessitate for development of cost effective, highly precise methods for early screening of HPV.<sup>15,16</sup> Also, screening aims to reduce cervical cancer incidence and mortality by the early detection of precancerous lesions that can progress to invasive cancers if undetected and untreated. Regrettably, the uptake of cytology-based screening (i.e., pap smear test) has fallen in recent years in the United Kingdom, with population coverage of 77.8% achieved in 2014 compared to 80.6% in 2004.<sup>17</sup>

In many low-income and middle-income earning countries (LMICs), no organized cervical cancer screening programs exist. Resourced screening is rarely offered because there is limited infrastructure to support current screening approaches using cervical cytology. In these countries, the detection of cervical cancer and precancer is mainly based on direct visual inspection. One advantage of the visual screening approach is the direct possibility of treating suspect lesions in the same session, the 'Screen and Treat' approach.<sup>18</sup>

Strategies for cervical cancer prevention and control in LMICs require concerted efforts to improve screening and access to treatment, especially in high-risk HIV populations. LMICs bear the largest burden of human immunodeficiency virus (HIV) infection while persistent high-risk HPV infection is more common among HIV-infected women. Thus, the risk of cervical cancer is increased in women with HIV/AIDS. HIV clinics provide opportunities to 'screen and treat' cervical precancer and cancer in this population.<sup>18</sup> This highlights the need for point-of-care HPV molecular diagnostics for a test and treat model in high-risk HIV populations. Implementation of the traditional Papanicolaou (Pap) smear in national screening programs is not sustainable in under-resourced LMIC settings with a limited skilled cytologist workforce<sup>20</sup> and where, despite a high prevalence of cervical cancer, lack of follow-up and poor adherence to treatment are major impediments for program success. The current World health organization (WHO) recommendation for HPV testing as a primary cervical cancer screening tool has been adopted by several countries such as Kenya, where it forms part of the national cancer screening guidelines.<sup>21</sup> However, it is difficult to detect small ectocervical and endocervical lesions under visual inspection (as in the case of Pap smear procedures). Depending

on the screening intervals, lesions might be overlooked and develop into invasive cancer. On the other side, many changes observed in visual inspection of the cervix with acetic acid (VIA) are rather non-specific and can result lead to substantial overtreatment of women. Treatment risks include haemorrhage, infection, obstetric complications including premature birth, cervical stenosis with failure to progress in labour and uterine rupture if not recognized, and increased susceptibility towards transmission of other sexually transmitted diseases (STDs), especially HIV.<sup>22</sup>

Besides high morbidity and mortality, another serious problem cancer is the widening of socioeconomic inequalities, with the most notable gaps for the most preventable cancers. For example, compared with the most affluent counties, mortality rates in the poorest counties were 2-fold higher for cervical cancer and 40% higher for male lung and liver cancers during 2012–2016.<sup>23</sup>

Current tumour diagnosis relies on various complex clinical settings, including X-ray imaging, computerized tomography (CT), magnetic resonance imaging (MRI), positron emission tomography, endoscopy, sonography, thermography, cytology and biopsy. In addition, molecular tools based on both genomic and proteomic are increasingly used, such as polymerase chain reaction (PCR), enzyme-linked immunosorbent assay (ELISA), radioimmunoassay (RIA), immunohistochemistry (IHC), and flow cytometry.<sup>24–26</sup> Of the existing technologies, most of them are invasive, expensive, time-consuming, and limited to laboratory centres in large hospitals.

Protein and nucleic biomarkers from body fluids such as tears, urine, sweat, saliva, and blood have been widely used in diagnosis and prognosis. Exosomes on the other hand are nano-sized bio-vesicles released into surrounding body fluids upon the fusion of multivesicular bodies and the plasma membrane. They were shown to carry cell-specific cargos of proteins, lipids, and genetic materials, and can be selectively taken up by neighbouring distant cells far from their release, reprogramming the recipient cells upon their bioactive compounds. Therefore, the regulated formation of exosomes, the specific makeup of their cargo, and their cell-targeting specificity are of significant biological interest. They are considered non-invasive diagnostic biomarkers, as well as therapeutic nanocarriers. As exosomes can be released by practically all eukaryotic cells, it is thought that their cargos may greatly differ from each other for the function of the originating cell types and their current state (e.g., transformed, differentiated, stimulated, and stressed). Thus, exosomes and their biologically active cargo may offer both diagnostic and prognostic information in a range of diseases, such as chronic inflammation,<sup>27</sup> cardiovascular and renal diseases,<sup>28,29</sup> neurodegenerative diseases,<sup>30</sup> lipid metabolic disease,<sup>31</sup> and tumours.<sup>32</sup>

This review investigates the different cancer biomarkers and techniques for detecting these biomarkers. The different point-of-care approaches for HPV detection and the current level of development of (POC) diagnostics devices are highlighted. However, a major concern with the existing HPV screen-and-treat approach is the overtreatment of high-risk HPV-positive women.

The review also explores other innovative point-of-care molecular diagnostic tools that are sensitive and specific using biomarkers that can serve both diagnostic and prognostic purposes in HPV screening which can be integrated into primary health settings in LMICs as screen-and-treat models. These point-of-care platforms can further be used to diagnose multiple conditions and monitor therapy on a single device.<sup>33</sup>

## CONVENTIONAL TECHNIQUES FOR HPV DETECTION

The conventional methods for the detection of HPV are well documented in<sup>34,35</sup> and may be categorized into four (**Figure 2**): (i) detection of the **morphology of the cell**, (ii) detection of **HPV genomes**, (iii) detection of **HPV Proteins**, and (iv) detection of **Anti-HPV antibodies**. Morphological changes in the cervix (e.g., precancerous, and cancerous lesions) arising from HPV infections are detected using the Papanicolaou stain (Pap smear), colposcopy, or by visual inspection analysis. Cytology or Pap smear represents the most successful HPV prevention worldwide as it has led to a significant reduction in cervical cancer and death. However, the main clinical drawbacks of the Pap smear are its low sensitivity, low specificity, and poor reproducibility.

It is not possible to culture HPV, so its accurate detection has mostly relied on molecular biology. The genome of HPV is well known to encode two early proteins (E1 and E2) that perform regulatory functions, two early proteins (E6 and E7) that carry out regulatory functions, and two late capsid proteins (L1 and L2). The role of protein E4 is not known, but protein E5 is hydrophobic and thought to improve cell immortalization. As shown in **Figure 2**, the use of HPV genomes for the detection of HPV infection and cervical cancer involves the use of the **Southern blot** analysis which is the gold-standard method for HPV genomic analysis. Southern blot methodology is time-consuming and requires significant amounts of purified DNA. Other methods in this category are in-situ hybridization, hybrid capture, and **real-time polymerase chain reaction (RT-PCR)**. Conventional PCR-based diagnostic tools are characterized by their high reliability, sensitivity, and specificity for the detection of HPV genotypes. Generally, these HPV genomes methodologies are characterized by their technical difficulty, time-consuming, and the need for DNA and tissue preservation. However, it provides information on the viral load.

Immunological-based detection of HPV is frustrated by certain challenges: (i) L1 and L2 are only expressed at the productive HPV infection stages; (ii) the early proteins (notably, the E1, E2, E6, and E7) proteins are expressed at very low levels in HPV infected cells, and (iii) the inability to produce high-quality antibodies that are sensitive and specific to the target HPV proteins. The detection of HPV proteins involves the use of immunohistochemistry (detection of L1 and L2 in squamous intraepithelial s), electron microscopy, and Western blot. In general, the detection of HPV proteins is characterized by low sensitivity, low specificity and can be cumbersome and time-consuming. The fourth method involves the detection of anti-HPV antibodies including ELISA peptides, the detection of virus-like particles (VLP), both of which have low sensitivity and specificity, and fused E6/E7. The pros and cons of these conventional detection techniques are summarized in **Figure 2**.

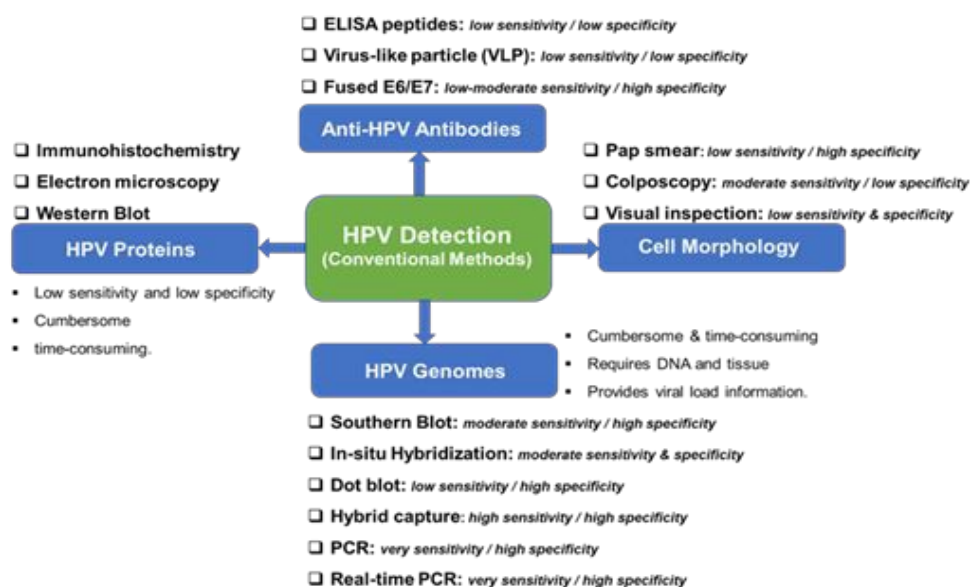


Figure 2: Conventional methods from the detection of HPV and their clinical sensitivity and specificity for CIN 2/3 lesions and cervical cancer

4 **Some recent efforts at improving the conventional HPV detection techniques**

7 **PCR Method**

8 Real-time polymerase chain reaction uses extracted DNA samples  
 9 that are subject to a real-time polymerase chain reaction (PCR) using  
 10 gene-specific primers, which target specific segments of the HPV  
 11 genome. In some modified PCR-based methods, messenger RNA  
 12 molecules (mRNAs) resulting from the transcription of genes E6 and  
 13 E7 are reverse-transcribed into complementary DNA, which in turn  
 14 is amplified in a PCR reaction. Oncoproteins E6 and E7 are the major  
 15 drivers of oncogenesis in infected individuals, and thus their  
 16 overexpression, detected at either the mRNA or protein level, is  
 17 predictive of the risk of developing cancer or may indicate  
 18 oncogenesis, regardless of the absence or presence of lesions. E6 and  
 19 E7 also drive tumor transformation. Melting curves are analysed  
 20 using the analysis program provided with the thermocyclers. We  
 21 positivity of HPV results, when analysed using PCR, are reported  
 22 negative results, therefore the need for an electrochemical method  
 23 which gives specific results. Alternative, to real-time PCR, which  
 24 prone to several short coming, droplet-digital PCR (ddPCR) is a  
 25 promising technique with improved sensitivity, elevated detection  
 26 rates and, does not require the use of standard calibration etc. The  
 27 ddPCR technique relies on the use of limited PCR volumes and  
 28 Poisson statistics. As a basis for this technique, samples are diluted  
 29 and partitioned in multiple reaction chambers or droplet. The  
 30 absolute quantity of PCR fragments is quantified from volume  
 31 water-in-oil droplet partition using the same standard PCR primers  
 32 and fluorescence probes, the absolute concentration is calculated  
 33 using Poisson statistics. This method has been used to  
 34 simultaneously detect and determine a numerous number of HPV  
 35 genotypes. Lv et.al. reported on the use of ddPCR for multiple

determination and quantification of HPV genotype among the  
 Chinese population, and the results showed high sensitivity,  
 specificity and accuracy compared to the traditional PCR [N. In  
 another study reported by Lillsunde Larsson et.al. ddPCR for a series  
 of high-risk HPV was studied, and later, ddPCR efficacy was  
 compared with traditional PCR for HPV 16 only and ddPCR showed  
 superior efficacy of 31:1 of traditional PCR. These studies show the  
 superiority of ddPCR compared to traditional PCR.<sup>36,37,38</sup> However,  
 the use of PCR methods for the detection of HPV is both labour-  
 intensive and cumbersome with the need for a highly skilled  
 technical expert for the interpretation of obtained results. In  
 addition, PCR tests do not provide evidence of past infection  
 therefore the natural course of the disease cannot be studied.<sup>39,40,41</sup>  
 The use of first void (FV) urine to test for HPV antibodies has shown  
 that there is “a good correlation between HPV 6, 11,16 and  
 18-antibodies in FV urine and paired sera, as well as between both  
 assays”, which confirmed that HPV-Abs originating from CVS are  
 detectable in FV urine of young women, although at low levels.<sup>42</sup> This  
 inadequacy limits the detection of the existing risk of developing  
 cervical cancer, especially in settings characterized by low  
 vaccination rates and limited prior HPV screening.

**DNA Microarray**

This is a laboratory tool used to detect the expression of thousands  
 of genes at the same time. DNA microarrays are microscope slides  
 that are printed with thousands of tiny spots in defined positions;  
 each spot contains a known DNA sequence or gene known as gene  
 chips or DNA chips. Each DNA molecule attached to each slide acts  
 as a probe to detect gene expression (transcriptome) or messenger  
 RNA (mRNA) transcripts expressed by a group of genes. First, mRNA  
 molecules are collected from both an experimental sample (an  
 individual with a disease like cancer) and a reference sample (a  
 healthy individual). The two mRNA samples are then converted into

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

complementary DNA (cDNA); each sample is labelled with a fluorescent probe of a different colour e.g. (cDNA) green, fluorescent dye while the experimental cDNA sample is a fluorescent dye. The two dyes are mixed for binding to occur which is known as hybridization; it is then measured to determine the expression of each gene printed on the slide. For the gene that expressed higher than the other, the colour will be high e.g., if it is experimental, the colour will be green but if both show equal expression, then the spot will appear yellow. The final data gathered can be used to create a gene expression profile in response to a particular treatment of the condition.

The susceptibility of the dye used in microarrays to the ozone effect makes it unstable in the presence of ozone which lowers the signal strength and prevents the scanner from recognizing it. Although it takes only a few minutes to convert the raw signal data of microarrays into high-quality data for further processing,<sup>43</sup> further analyses can be done using different in-house software packages such as PePPER, FIVA, DISCLOSE, PROSECUTOR.<sup>44-47</sup> This is followed by result verification which can be done using qPCR or  $\beta$ -galactosidase assays using *lacZ* promoter fusions.

Gogianu et al.<sup>48</sup> reported the use of carbon dots for the first time to increase DNA microarray biochips' detection performance, the authors achieved a fluorescent hybridization intensity of 3.744 for HPV 16. Recently, Varesano et al.<sup>49</sup> combined the use of HPV 16/18 genotyping and microRNAs detection, as a triage test for HPV positive women to identify subjects at high risk for cancer progression.

### Immunology-Based Method

Three serological assays commonly used in clinical trials for the detection of HPV antibodies are HPV pseudovirion-based neutralization assay (PBNA), competitive or total Luminex immunoassays (cLIA or LIA) and VLP-based enzyme-linked immunosorbent assays (ELISA).<sup>50</sup> The gold-standard method is PBNA which has the following drawbacks: difficult to set up, laborious, and does not discriminate between different antibody isotypes and subclasses. As for cLIA/LIA and VLP-ELISA, they have high throughput and are rapid; but their reagents and equipment are difficult to source. However, the standard good laboratory practices which sometimes give a false positive result in the laboratory must be addressed especially when performing analysis of samples from the same individuals on the same plate as, the pre- and post-samples, which will eliminate both inter-plate variations and appropriate controls, i.e., pooled serum controls.<sup>41</sup> Furthermore, the traditional antibody-based methods may not be sensitive enough to detect the infection

in the early stages, especially because the expression of viral proteins may be low during this period, requiring a more sensitive method for the detection of low-abundance proteins. The antibody-based detection methods of E6 and E7 mRNAs hybrids with specific DNA probes have been developed and reported. The authors revealed that the method detects E6 and E7 mRNA without the costly amplification of nucleic acids, rather with the use of the S9.6 antibody and horseradish peroxidase (HRP)-linked secondary antibody.

### EMERGENT TECHNIQUES FOR HPV DETECTION

The limitations of the conventional HPV detection techniques have informed the need to explore other techniques that would allow for sensitive, specific, fast detection, and low cost. Some of the emergent diagnostic tools include the Fourier transform infrared spectrophotometry (FTIR), Raman spectroscopy and surface-enhanced Raman scattering (SERS), mass spectrometry, and electrochemical methods. As the readers will see later, of all these methods, electrochemical methods have received much attention.

#### Fourier transform infrared spectrophotometry (FTIR)

Fourier transform infrared spectroscopy can potentially improve clinical decision-making and patient outcomes by detecting biochemical changes in cancer patients at the molecular level. It is more simple, more rapid, more accurate, inexpensive, non-destructive, and suitable for automation compared to existing screening, diagnosis, management, and monitoring methods.

There are three regions for the infrared spectrum: near-infrared (NIR) in the 0.76–2.5  $\mu\text{m}$  (12,500–4000  $\text{cm}^{-1}$ ) region, mid-infrared (MIR) in the 2.5–25  $\mu\text{m}$  (4000–400  $\text{cm}^{-1}$ ) region, and far-infrared in the 25–1000  $\mu\text{m}$  (400–10  $\text{cm}^{-1}$ ). The most used region for biological applications is MIR, which consists of the fingerprint region of 1800–900  $\text{cm}^{-1}$  for proteins (amide I/II/III), lipids, carbohydrates, and nucleic acids. NIR spectroscopy may be used in similar applications to MIR spectroscopy. NIR spectra are occupied by overtone (resonant bands above the fundamental bands) and combination bands with the typical absorption coefficients two orders of magnitude lower than that of MIR fundamental bands. Therefore, NIR light can penetrate much deeper into the sample surface than MIR light, which makes NIR spectroscopy better suited for deep tissue sampling and the examination of highly moist specimens.

FTIR records spectrochemical information composed of the absorption intensities for each wavenumber of the mid-infrared spectrum (4000–400  $\text{cm}^{-1}$ ).


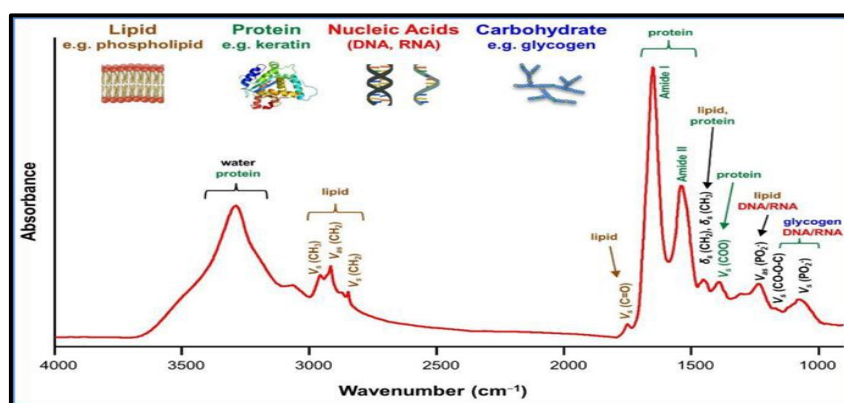


Figure 3: Common Fourier transforms infrared (FTIR) bands for biomolecules<sup>51</sup>

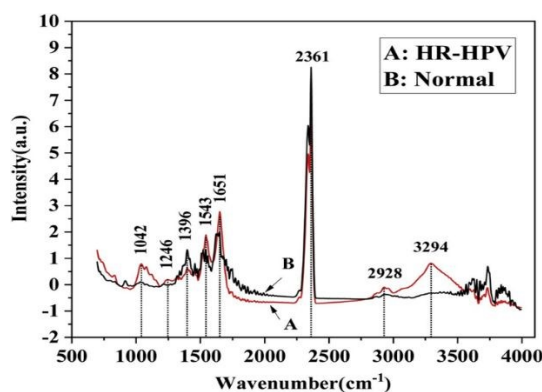

**Figure 4:** Normalized mean FT-IR spectra of HR-HPV positive patients and normal people (The red solid line (A) is the FT-IR spectra of cervical exfoliated cells of 50 HR-HPV positive patients, and the black solid line (B) is the FT-IR spectra of cervical exfoliated cells of 50 normal people).<sup>60</sup>

The infrared bands carry vibrational information used to identify the molecular components and their respective structures; thus, the spectra generate a distinctive molecular fingerprint used to screen and scan samples in various segments. The fingerprint spectrum of biological samples also called the “bio fingerprint” region ranges from 1800 to 900  $\text{cm}^{-1}$  as shown in Figure 3<sup>51</sup> and contains information on key biomolecules such as lipids, proteins, carbohydrates, and nucleic acids<sup>52</sup>. Changes in the IR signature of these biomolecules are associated with concentration changes (changes in band intensity) and changes in molecular configuration and neighbouring functional groups (band shifts towards higher and lower wavenumbers). Thus FT-IR generates chemically rich spectral signatures of tissue or biofluids that can be used for a wide range of clinical applications, especially in oncology.<sup>53</sup>

FTIR has been reported as a non-invasive method for the detection of HPV.<sup>54-61</sup> For example, Mo et al.<sup>60</sup> employed FTIR as a non-invasive method to detect HR-HPV in patients. A total of 100 spectra were recorded from 50 HR-HPV-positive patients and 50 normal subjects. They found clear differences in the recorded spectra of the two groups (Figure 4). Unlike the normal subjects, the spectra of the HR-HPV patients showed peaks at the 1042  $\text{cm}^{-1}$  (mucin), 1246  $\text{cm}^{-1}$  (amide III), 1396  $\text{cm}^{-1}$  (proteins), 1543  $\text{cm}^{-1}$  (amide II), 1651  $\text{cm}^{-1}$  (amide I), 2361  $\text{cm}^{-1}$  ( $\text{CO}_2$ ), 2928  $\text{cm}^{-1}$  (lipids), and 3294  $\text{cm}^{-1}$  (amide I).

The sensitivity of FTIR spectroscopy to chemical changes during the transition from normal to pathological state or during treatment can lead to the identification of novel biomarkers associated with disease.<sup>62,63</sup> In situ chemical composition analysis of cirrhosis combining synchrotron Fourier transform infrared and synchrotron X-ray fluorescence spectroscopy on the same tissue section}. However, some authors<sup>57,58,61</sup> have suggested FTIR spectroscopy considered a complementary diagnostic method to PCR, cytology, immunofluorescence, molecular histopathology, and other methods.

#### Raman Spectroscopy and Surface-Enhanced Raman Scattering (SERS)

Raman spectroscopy has emerged as an important technique for the detection of various types of pathologies, including cervical cancers.<sup>64-73</sup> It has been used in understanding the progression of the disease at the molecular level. The Raman spectrum of any sample acquired by simply irradiating the sample with a laser source

either visible or near-IR monochromatic irradiation) and then measuring the scattered radiation with an appropriate spectrometer. Since every molecule exhibits highly specific and distinctive spectral features, a Raman spectrum can serve as a crucial identification marker for a particular sample. Figure 5A depicts a typical full Raman spectrum of a cervical cancer cell line, CaSki.<sup>64</sup> It shows characteristic features in the fingerprint (400 - 1800  $\text{cm}^{-1}$ ) and high wavenumber (2800 - 3500  $\text{cm}^{-1}$ ) regions. Figure 5B is the expanded fingerprint region, highlighting the major assignments that are associated with glycogen, proteins, lipids, and nucleic acids. Surface-enhanced Raman scattering (SERS) is an ultrasensitive analytical vibrational spectroscopic technique. The enhanced SERS signal is attributed to the combined electromagnetic and chemical effects. The ability to generate high Raman signal by this technique is mostly dependent upon the SERS-active substrates used, most preferably the bimetallic nanomaterials such as gold-silver (Au-Ag) materials. Many researchers have adopted bimetallic Au-Ag nanomaterials for SERS because of the inherent advantages of generating stronger and sharper surface plasmon resonance and excellent SERS activities compared to the monometallic counterparts. Recently, Ning et al.<sup>74</sup> reported the ultrasensitive detection of HPV-16 using specific oligonucleotides based on Au@AgAg bimetallic nanorods.

#### Clustered regularly interspaced short palindromic repeats (CRISPR)-


Clustered regularly interspaced short palindromic repeats (CRISPR)-based assay is an emerging technology that has found application in the sensitive detection of pathogens.<sup>75-86</sup> CRISPR is a gene editing technique, that can be used to edit genes with mutation or be used to cure some diseases. CRISPR consists of two important components: the guide RNA (gRNA) and Cas9 protein. The gRNA acts as a guide by identifying DNA target while Cas9 protein cuts the identified DNA target. The gene editing consists of several essential steps. Firstly, the gRNA identifies the target DNA, after which the Cas9 protein cleaves the targeted DNA. This is followed by the repairing step at the target site through the non-homologous end joining (NHEJ) or homology-directed repair (HDR) pathways. Two approaches can be used for gene editing i.e. the single and multiplex approach. In the single approach, the single guide RNA directs the Cas protein to a single target DNA where it binds and cleaves the target DNA after which editing of the gene occurs, while the multiplex approach involves the sgRNA identifying multiple target DNA, and the Cas protein cleaving multiple DNA targets, after which

simultaneous DNA editing occurs.<sup>87-89</sup> A new strategy that involves the combination of CRISPR and SERS has also emerged and proving to be a hot topic due to its extraordinary sensitivity.<sup>77,90-93</sup> For example, Choi et al.<sup>94</sup> reported the use of the CRISPR/SERS system to enhance the detection of HPV-16 and HPV-18 to an extremely low detection limit (i.e., atto-Molar concentration level) at a very short time of 20 minutes. Su et al.<sup>95</sup> used CRISPR/Cas-SERS to detect HPV genes

in serum with a very low detection limit in the pico-Molar concentration level.

DOI: 10.1039/D4AY01921K

CRISPR/Cas SER-based technology holds great promises in HPV diagnosis, and as attested by recent authors,<sup>96-98</sup> its good sensitivity and specificity need to be further explored in complex biological environments using minimally invasive samples such as biofluids (blood, urine) or exfoliated cells on larger patient cohorts.

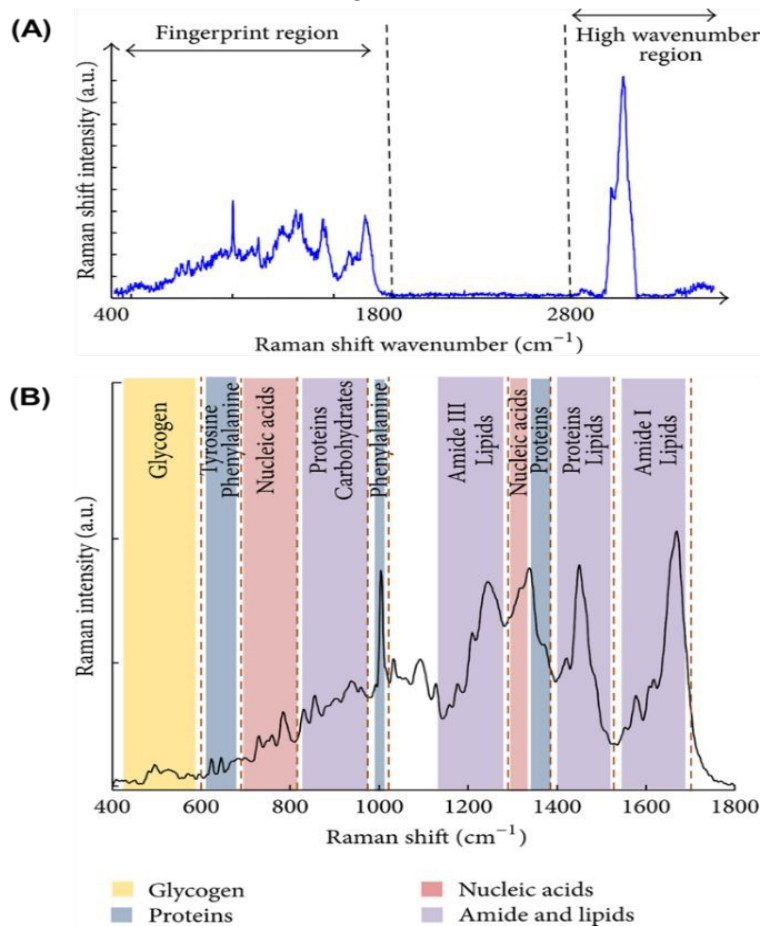

**Figure 5:** (A) Raman spectrum of cervical cancer CaSki cell line. The variation of Raman shift wavelength is expressed in wavenumbers ( $\text{cm}^{-1}$ ) and can be observed along the  $X$ -axis whilst the intensity is represented along the  $Y$ -axis. The fingerprint and the high wavenumber (HW) regions of the spectrum are indicated by the arrows. (B). Fingerprint region of the Raman spectrum of cervical cancer CaSki cell line. The major assignments related to glycogen, proteins, lipids, and nucleic acids are highlighted.<sup>64</sup>

## Mass Spectrometry

Mass spectroscopy (MS) determines the molecular mass of a charged particle by measuring its mass-to-charge ( $m/z$ ) ratio. A mass spectrum is a plot of ion abundance versus  $m/z$ . A mass spectrometer consists of an ion source that converts molecules to ionized analytes, a mass analyser that resolves ions according to the  $m/z$  ratio, and a detector that registers the number of ions at respective  $m/z$  values. The mass analyser depends on three key parameters: sensitivity, resolution, and mass accuracy. The sensitivity, resolution, and accuracy of advanced mass spectrometers allow the detection of femtogram levels of individual proteins in complex mixtures. Recognized by the 2002 Nobel Prize in Chemistry, innovation in electrospray ionization (ESI) and matrix-assisted laser desorption/ionization (MALDI) techniques has made it possible to ionize big molecules such as proteins, peptides, and nucleotides for mass spectrometric analysis. ESI generates ions at atmospheric

pressure by injecting a solution-based sample through a small capillary. MALDI produces ions by pulsed-laser irradiation of a sample that is co-crystallized with a solid matrix that can absorb the wavelength of light emitted by the laser. Protonation or deprotonation is the main source of charging for the ions generated in ESI/MALDI.<sup>99</sup>

Mass spectroscopy imaging, MSI is mostly used in cancer research and consequentially for oncogenic viruses. Different MSI-based techniques, alone or in combination with various other proteomic and imaging approaches have been successfully applied to study virus infections, virus-induced tumours, and antiviral compounds. It provides molecular information on a large variety of analytes including their spatial distribution. Therefore, this label-free imaging approach is a promising option for the analyses of tissues and cells in biomedical research.<sup>100</sup> Schwamborn et al.<sup>101</sup> reported the combination of traditional morphology analyses and cytological evaluation with MALDI MSI-derived molecular signatures to facilitate






the automated diagnosis and stratification of high-risk HPV-derived cervical carcinomas into different cervical Papanicolaou (Pap) classes using cytospin preparations of Pap smears. The authors were able to screen and classify cervical cytology samples and simultaneously diagnose HPV infections routinely and in an automated manner using this feasible approach. Godoy-Vitorino et al.<sup>102</sup> recently reported a study on the detection of HPV+H infections in urine, via analysis of some urine metabolites using just 200  $\mu$ L of the urine sample. The metabolite separation was done by Gas Chromatography and detection by Mass Spectroscopy. The study provided preliminary evidence for the successful detection of urine metabolites related to cervical high-risk HPV infections. The GC-MS analysis showed that patients with high-risk HPV infections have a significantly higher abundance of 5-Oxoprolinate, Erythronic acid, and N-Acetylaspartic acid. Besides characterizing cervical HPV, the authors were able to relate high-risk HPV infections with urinary metabolites and defined 5-Oxoprolinate, Erythronic acid, and N-Acetylaspartic acid as possible prognostic biomarkers for high-risk HPV infections. MS-based proteomics analyses of complex protein mixtures have also been reported.<sup>103</sup> They usually require a starting amount in the range of 0.1–10  $\mu$ g, depending on the experimental setup and the type of mass spectrometer used. In contrast to other standard

techniques, MSI is neither restricted to one or more defined analytes nor limited by the availability of antibodies, fluorescent chromophores, or nucleic acid probes. Furthermore, MSI techniques are highly versatile and specific at the same time, as numerous masses can be simultaneously detected and discriminated.

### Electrochemical Methods

Electrochemical biosensors are very important alternative tools to other detection methods for pathogens, including cervical cancers. As shown in **Figure 6**,<sup>104</sup> electrochemical biosensors are characterized by several unique advantages, including fast response time, simple to use, low cost, easy to miniaturize, highly sensitive, and selective. These advantages are important for cervical cancer detection. For example, the ability of the electrochemical biosensors to give an ultra-low limit of detection is crucial because the concentration of the cancer biomarkers is very low in their early stages.<sup>105</sup> A typical electrochemical biosensor comprises two main components. The transducer is made up of two components: the bioreceptors and the interface (transducer). Both serve as recognition probes for target analytes. Table 1 also shows commonly adopted methods for the detection of HPV.

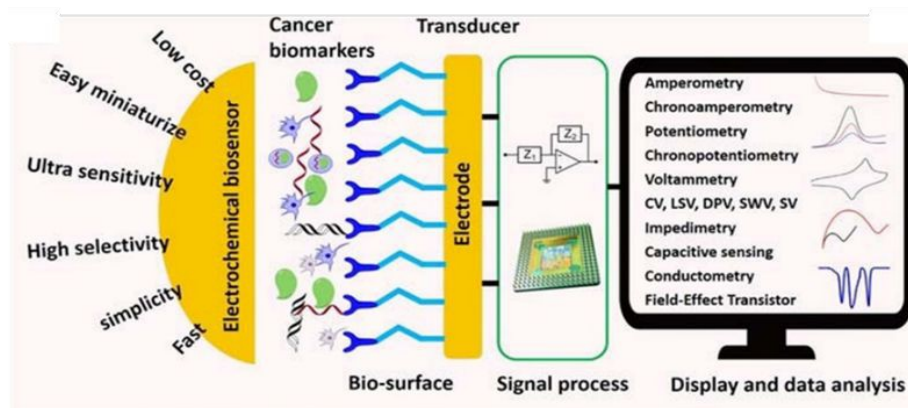


**Figure 6:** Schematic diagram of advantages, component parts, and various measurement methods of electrochemical biosensor.<sup>104</sup>

Some recent developments in electrochemical biosensing include the discovery of bioreceptors with high specificity and affinity, the design of novel redox tags to conduct multiplex bioassay and ratiometric electrochemical assay, the development of signal amplifiers based on nanomaterials, and the integration of electrochemical biosensors with microfluidic chips.<sup>106,107</sup> The receptor is the most important component for the design of an electrochemical biosensor, which involves antibodies, lectins, peptides, deoxyribonucleic acid (DNA), peptide nucleic acids (PNA), aptamers, molecularly imprinted polymers (MIPs).<sup>104,108</sup> It is the biosensing element to which the analyte has a highly specific binding affinity. Antibodies (immunoglobulins) are immune system-related proteins, which can selectively bind to antigens with a high binding constant of more than  $10^8$  L mol<sup>-1</sup>. The significant advantage of antibodies is the specificity and affinity of these probes to target analytes. Electrochemical biosensors can provide fast, accurate, sensitive early detection, measure and analyse the effectiveness of anticancer chemotherapy drugs in a non-invasive style and monitor cancer metastasis and angiogenesis. It will be a strong candidate for cancer theranostics because it possesses the advantages of high selectivity, low cost, ultra-sensitivity, simplicity, easier of be miniaturized, and mass fabrication which grant them a better fit for point-of-care (POC)

devices at home or clinic.<sup>109</sup> Such a method can be developed based on an antibody reacting with either the E6 or E7 oncoproteins, whose detection can reveal the level of risk for developing HPV-induced cervical cancer. The method was previously reported for the detection of cholera, based on an antibody-probe system detecting cholera toxin as the target antigen.<sup>110</sup> It is therefore plausible to presume that such a method can be adapted for the diagnosis of HPV infection directly via the detection of HPV-derived oncoproteins, or indirectly by detection of host proteins affected by interaction with these oncoproteins, such as tumour suppressor p53 and cell cycle checkpoints. The latter strategy may only give evidence of the extent of the infection and the development of cancer.

Electrochemical biosensors play a crucial role in the development of point-of-care (POC) diagnostics because they are simple to use, rapid, real-time, cost-effective, and easy to miniaturize and mass-produce. They also can be used as point-of-care (POC) devices at home or doctor's office. Therefore, they have received significant attention, and extensive efforts have been devoted to developing ultrasensitive electrochemical biosensors for the detection of cancer markers with high selectivity.<sup>111</sup> For example, the publication rate in electrochemical detection of HPV grew steadily from 2019 to 2023 (**Figure 7**).

## ARTICLE

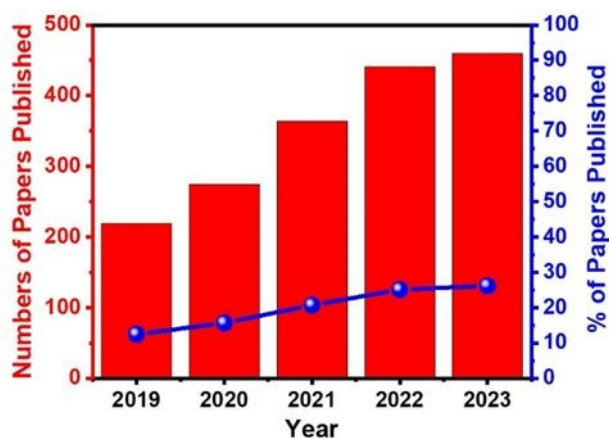

**Figure 7:** Percentages of papers published on electrochemical detection of cervical cancer / HPV from 2019 to 2023 (Google Scholar database, keywords “electrochemical analysis of cervical cancer, electrochemical detection of HPV”)

**Table 1:** Summary of traditional methods used for HPV detection.<sup>112</sup>

	Detection method	Pros	Cons
<b>DNA level</b>	PCR	Simple, quick Sensitive Highly specific	Easy to cross-contamination between samples High false positive rate Perform HPV typing operations is tedious
	DNA ISH	High specificity Can be used for localization detection	Detection is affected by the DNA content in the specimen Results are sometimes difficult to explain
<b>mRNA level</b>	RT-PCR	High sensitivity High specificity Accurately reflects the transcription activity of viral oncogenes	Requires technical expertise Testing fresh frozen tissue
	RNA ISH	High sensitivity High specificity To some extent, it can be used as the "gold standard" for HPV-related tumors	The experimental operation requires high experience Poor repeatability
<b>Protein level</b>	p16 immunohistochemistry	High sensitivity Strong prognostic indicators	Low specificity Mainly used for the detecting HPV in oropharyngeal cancer
	IHC	Virus antigen detection Easy to perform and locate	False-negative findings and low sensitivity

The electrochemical biosensor<sup>113</sup> measurement depends on the impulsive interaction between a chemical reaction and electrical energy that involves an oxidation–reduction reaction to generate electrical current or vice versa. The chemical process that occurs between immobilized biomaterials and the analytes caused production/consumption of ions or electrons, that affect electrical current, the electrical potential, or any other electrical property of the solution. These reactions occur at metal/semiconductor electrode and an electrolyte interface. Thus, detection is feasible if the reactions occur in close contact with the electrode surface. Hence, the electrodes significantly influence the performance of the electrochemical biosensor. One must consider several factors when choosing a proper electrode, including its material, dimension, and possibility to carry out surface modifications. Most electrochemical cells are composed of three electrodes (**Figure 8 (A)**): (1) a reference electrode (RE), which is

usually Ag/AgCl and positioned at a distance from where the reaction takes place. This is to provide a potential that is proportional to the known and stable solution. Furthermore, the RE allows normalization of the measurements. (2) A counter electrode (CE), also known as auxiliary electrode is the source of the current that is afterwards applied to the working electrode. (3) A working electrode (WE) which is the sensing or reduction/oxidation electrode. The WE acts as a transducer in the biochemical reaction. The CE and WE should be

chemically stable and conductive. Therefore, the main electrode materials used are gold, silver, platinum, silicon, carbon and graphene depending on the analyte and the nature of the reaction. The screen-printed electrode (SPE) (Figure 8 (B)) is an alternative to the electrochemical cells used in electrochemical sensors. The SPE is a version where the three electrodes are screen printed on an insulating substrate. The SPEs have several advantages of simplicity, scalable, low-cost and low analyte/reagent consumption.

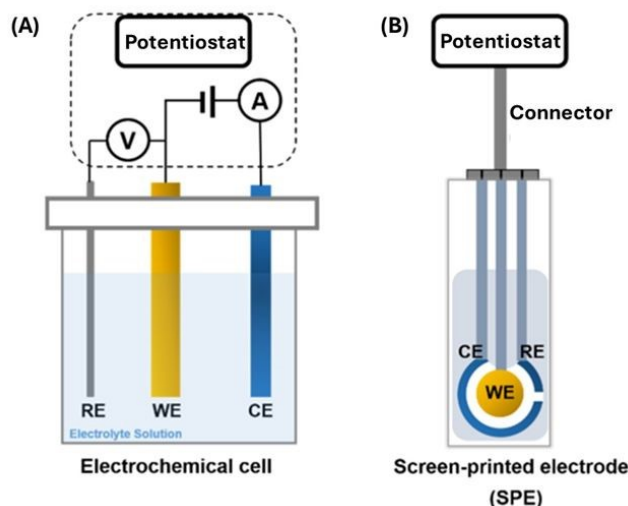


Figure 8: Electrochemical sensors – three electrodes system (A) electrochemical cell (B) screen printed electrode (SPE)<sup>113</sup>

Table 2: Different types of biosensors, their shortcomings and advantages.<sup>120</sup>

Biosensor	Types	Advantages	Disadvantages	Solution
Electrochemical	Amperometric, potentiometric, conductimetric, impedimetric and voltametric	Excellent detection limits, faster detection, ease of fabrication, good resolution, linear output	Unstable current and voltage, limited/narrow range, short/limited shelf life, cross sensitivity with other gases	Design and employ electrocatalysts that are stable to minimize unstable currents and voltage
Optical	Surface plasmon resonance (SPR), fluorescence, bio/chemiluminescence, refractive index, Raman scattering, absorbance	High sensitivity, selectivity, cost-effectiveness, small size	Susceptible to physical change and interference from environmental effects	Use material that are stable in a wide range of temperatures
Thermal/calorimetric	Thermistors or thermopiles	Scalability, Ease of use and ease of fabrication	Lack of specificity in temperature measurements, long experimental procedures	Use high sensitivity thermocouple
Mass sensitive or gravimetric	Wave biosensor, surface acoustic, cantilever	Low cost and simplicity	Low sensitivity	Employ materials with high sensitivity to mass changes, such as piezoelectric materials or graphene
Piezoelectric	Surface acoustic devices, Piezoelectric crystal	Fast detection, good frequency response, small size and high sensitivity	High temperature sensitivity, not suitable for static conditions, some crystal can dissolve in high humid environment and are water soluble	Maintain humid controlled environment and use water repellent coating

Antibody-based electrochemical biosensors, (electrochemical immunosensors) are one of the most common biosensors for cancer protein biomarkers detection.<sup>114,115</sup> Lectins are natural proteins of non-immune origin with specific binding affinity for the glycan

moiety of glycolipids and glycoproteins. They are valuable recognition elements for the biosensing of glycoprotein tumour markers.<sup>116</sup> Peptides are short chains of amino acid monomers linked by amide bonds. They represent a promising class of biorecognition

Open Access Article. Published on 23 December 2024. Downloaded on 16/2025 5:31:52 PM. This article is licensed under a Creative Commons Attribution 3.0 Unported Licence.




elements that can be coupled to electrochemical transducers. Compared to antibodies, they are more stable in harsh environments and selectivity toward a target analyte. Furthermore, they can be synthesized easily and modified with specific functional groups, thus making them suitable for the development of novel architectures for biosensing platforms. Peptides have also been proposed as anti-biofouling agents.<sup>117</sup> Deoxyribonucleic acids (DNAs) are stable, low-cost, and easily adaptable molecules. They have been employed to build a variety of biosensors via the interactions between DNAs and biomolecules or chemical compounds, with high sensitivity and selectivity. DNA-based label-free electrochemical biosensors, without additional assay reagents and tedious procedures, have also attracted tremendous attention from researchers and have been seen as promising analytical technology due to their simplicity.<sup>118</sup> DNA-based electrochemical detection of HPV is the highly sensitive and specific method for the detection of HPV.<sup>119</sup> In this case, the probe DNA is first immobilized on the electrode surface, then used to hybridise with the target complementary HPV DNA. The hybridization is detected by measuring the electrochemical signal response using any of the electrochemical techniques (such as SW-DPV, EIS, etc). The most important part of electrode fabrication is the ability to immobilize the probe DNA on the electrode surface.

### Immobilizing the HPV probe onto the electrode surface: Some chemistry-inspired tricks

DOI: 10.1039/D4AY01921K

Immobilization of the HPV probe or the recognition element onto the electrode surface is the most critical step in the development of the immunosensor. If the probe (i.e., antigen, antibody, DNA, or RNA) is properly oriented on the electrode surface, there is a high chance that the performance of the immune sensor would be improved. There are three chemistry-inspired tricks that one can adopt in immobilizing the probe onto the electrode surface, viz: (i) **ionic bonding**, (ii) **covalent bonding** (i.e., **amide bond creation**), and (iii) **self-assembly** (or **chemisorption**) process.

The **ionic bonding** technique may be exemplified by the work of Teengam et al.<sup>121</sup> who fabricated an HPV DNA sensor by first generating a positively charged amino group surface using polyaniline (PANI, emeraldine base) doped with camphor-10-sulfonic acid (CSA) that can coordinate with a negatively charged target DNA probe (**Figure 9**). To obtain a negatively charged DNA probe, the authors modified the DNA probe with glutamic acid residues at the N-terminus to generate the negative charge, followed by end-capping with an acetyl group.

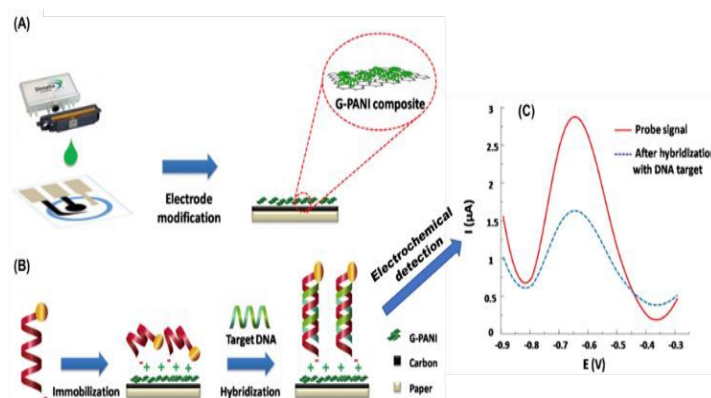

**Figure 9:** Schematic illustration of (A) electrode modification and (B) immobilization and hybridization steps of paper-based electrochemical DNA biosensor. (C) Square-wave voltammograms of immobilized AQ-PNA probe on G-PANI/SPCE before and after hybridization with an equimolar concentration of target DNA.<sup>121</sup>


Another way by which ionic bonding can be created is the electrodeposition technique. Pareek et al.<sup>122</sup> proposed an electrochemical biosensor comprising an indium tin oxide (ITO) coated glass modified with electrodeposited graphene oxide nanoribbons (GONR) and silver-coated gold nanoparticles (Ag@AuNPs) as the electrode for the immobilization of the probe DNA (PDNA) as a sensor for the target DNA (TDNA) of the HPV-16 (**Figure 10**). The stability of the sensor was attributed to the electrostatic interaction between the negatively charged phosphate backbone of the PDNA and the positively charged nanomaterials (GONRs/Ag@AuNPs). The sensing activity was studied using CV and EIS. The proposed biosensor exhibited excellent sensitivity (0.82 mA/aM) and low detection limit of 100 aM. The **amide bond formation** is the conventional technique for immobilizing antibodies or antigen-based probes. This technique is famous for immobilizing antigens and antibodies. However, since DNA contains amino terminal groups, it is also possible to adopt the amide-bonding technique. The process uses 1-Ethyl-3-(3-dimethyl aminopropyl

carbodiimide hydrochloride (EDC) and N-hydroxy succinimide (NHS). The EDC/NHS activation approach possesses many merits which include high conversion efficiency, mild reaction conditions, excellent biocompatibility with little influence on the bioactivity of target molecules, and much cleaner products than other crosslinking reagents.<sup>123-126</sup> The more water-soluble derivative of NHS-hydroxysulfosuccinimide (Sulfo-NHS) /EDC has also been used as a molecular linker to immobilize the DNA probe on the graphite-based substrate.<sup>110,127,128</sup> Alternatively, one can utilize 1-pyrenebutyric acid-N-hydroxysuccinimide ester (PBSE) as adopted by Asadi et al.<sup>129</sup> for the detection of microRNAs (miRNA-21) which is a potential prostate cancer biomarker.


The **self-assembling** process benefits from the strong affinity that exists between gold and sulphur-based molecules or thiolates that leads to the formation of a self-assembled monolayer (SAM). It is not surprising therefore that SAMs are formed on gold electrodes. Recently, Wang et al.<sup>130</sup> encapsulated an anti-HPV-16 L1 monoclonal antibody on a gold electrode by using *Staphylococcal* protein A (SPA),

1 instead of the conventional grafting technique that utilizes EDC/NHS  
 2 for the sensing of antigenic HPV-16 L1 (Figure 11). SPA is found on  
 3 the cell of the *Staphylococcus aureus* and is said to contain four  
 4 active sites that can easily bind with the non-antigenic Fc receptor  
 5 (i.e., fragment crystallizable) portion of the immunoglobulin G (IgG),

thus allowing the antigen-binding region (i.e., fragment antigen-binding) portion to be properly exposed to the surface for easy binding with the target antigens.

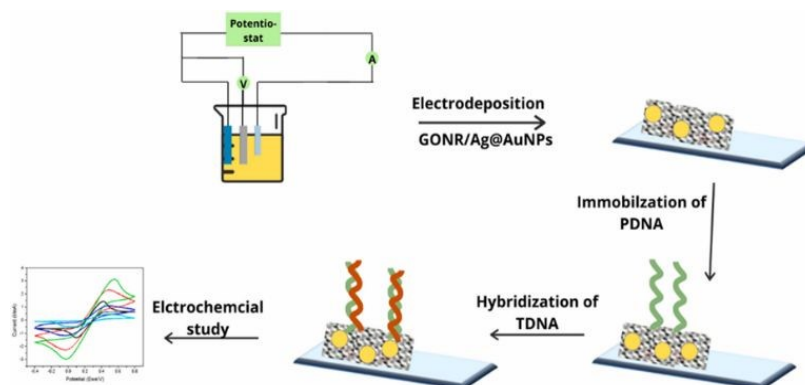

**Figure 10:** Stepwise representation of the encapsulation onto the ITO surface with GONR/Ag@AuNPs and probe DNA (PDNA) for electrochemical detection of the HPV target DNA (TDNA).<sup>122</sup>

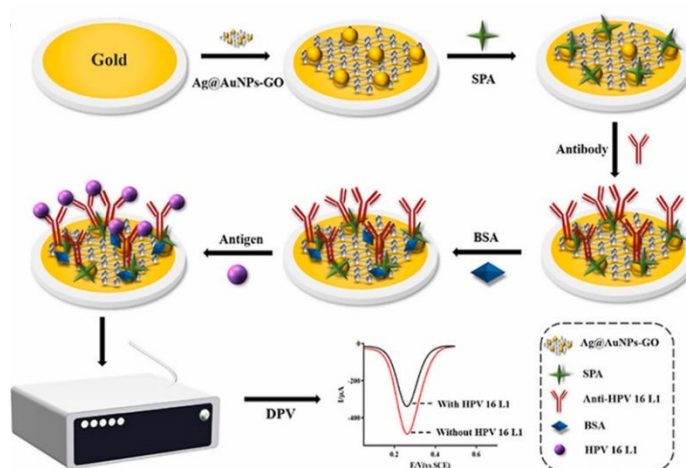

**Figure 11:** Stepwise encapsulation of Ag@AuNPs-GO, SPA and anti-HPV-16 L1 antibody onto the gold electrode surface for the electrochemical detection of the target antigenic HPV-16 L1 protein.<sup>130</sup>

23 As shown in Figure 6, several electrochemical techniques can be used  
 24 for the detection of cancer biomarkers. The most important  
 25 techniques are voltammetry (such as square wave voltammetry  
 26 (SWV) and differential pulse voltammetry (DPV)) and Impedimetric  
 27 technique. Impedimetric techniques have been proven to be a  
 28 promising method for cancer biomarker detection due to their low  
 29 excitation voltage, fast speed, and high sensitivity. They can be used  
 30 for long-time, real-time, and on-site detection. Electrochemical  
 31 impedance spectroscopy (EIS) is the most often used impedance  
 32 method for electroanalytical detection<sup>131-136</sup> is a high-sensitivity, low  
 33 cost, fast, label-free, and minimally invasive method for recording  
 34 biological events. It uses an amplitude sinusoidal AC excitation signal  
 35 typically in the range of 2–10 mV, to determine the measurement  
 36 resistance and capacitance characteristics of materials that adsorb  
 37 the electrode surface. The low excitation voltage makes it become a

safer detection technology for bioelectrochemical analysis systems  
 that require long-term monitoring. As electrode heating is a problem  
 that can cause changes in the biological microenvironment and  
 damage to the electrodes, low excitation voltage does not generate  
 a lot of heat, hence EIS is more suitable for long-term and real-time  
 detection. Additionally, the EIS provides multiple parameters of the  
 biosensing surface. Using a redox couple, typically a mixture of  
 ferricyanide and ferrocyanide, the change in the charge transfer  
 resistance ( $R_{ct}$ ) is obtained. Usually, the  $R_{ct}$  is inversely proportional  
 to the rate of electron transfer. The double layer capacitance ( $CPE$ )  
 and the  $R_{ct}$  describe the dielectric and isolation features of the  
 electrode-electrolyte interface. The electrolyte resistance ( $R_s$ ) and  
 the Warburg impedance ( $Z_w$ ) characterize the properties of an  
 electrolytic solution and diffusion limitation for the redox probe to  
 reach the electrode surface and do not affect electron transfer at the

electrode surface. The detection in the broad frequency range (10<sup>3</sup>–10<sup>6</sup> Hz) makes the EIS strategy useful for diffusion analysis and providing kinetics characteristics. Generally, at low frequencies (f < 100 kHz) the impedance is determined by the DC-conductivity of the electrolyte solution, and at higher frequencies (f > 100 kHz), the inductance of the electrochemical cell and connecting wires dominate the system.<sup>137,138,139</sup>


**Field-Effect Transistor (FET)** based biosensors measure the conductivity of a channel (i.e., region depleted of charge material) between two electrodes (the source and drain) in FET (semiconductor) devices, see Figure 12 for experimental illustration. Once the probe binds its analyte molecule, the electric field of environment alters, thus producing a measurable change in source-drain conductivity.

In recent years, several FET techniques have been reported for sensitive and selective detection of HPV.<sup>140–144</sup> For example, Aspermaier et al.<sup>140</sup> reported the use of rGO-FET for ultrasensitive and selective detection of HPV-16 E7 protein. The high performance of this sensor was attributed to attractive semiconducting characteristics of pyrene-modified rGO functionalized with RNA aptamer Sc5-c3. The aptamer-functionalized rGO-FET allows monitoring the aptamer-HPV-16 E7 protein binding in real-time with a detection limit of about 100 pg mL<sup>-1</sup> (1.75 nM). The authors successfully demonstrated the feasibility of this rGO-FET sensor for clinical application in point-of-care technology. HPV DNA and human telomerase reverse transcriptase (hTERT) mRNA are important biomarkers for cervical cancers because of their high levels of expression in cervical cancer cells, but little or no expression in

normal cervical tissue. Some workers<sup>141</sup> demonstrated the efficacy of a handheld Lab-on-Chip (LoC) device, based on an Ion-Sensitive Field-Effect Transistor (ISFET) sensor, in detecting cervical cancer from biopsy samples. The device was combined with loop-mediated isothermal amplification (LAMP) assays with the objective of amplifying the HPV DNA and hTERT mRNA.

Gao et al.<sup>142</sup> fabricated a nanomaterial-based field transistor (FET) sensor made with the polyethylene glycol (PEG)-modified graphene device that exhibited real-time reversible detection of prostate-specific antigen (PSA) from 1 to 1,000 nM in 100mM phosphate buffer. Lu et al.<sup>143</sup> also developed a complementary metal oxide semiconductor (CMOS)-compatible SiNW-FET biosensor fabricated by an anisotropic wet etching technology. They reported a rapid (< 1 minute) detection of miR-21 and miR-205, with a low limit of detection (LOD) of 1 zeptomole (ca. 600 copies), as well as excellent discrimination for single-nucleotide mismatched sequences of tumor-associated miRNAs.

Compared with other traditional clinical diagnostic tools, the electrochemical techniques display sensitivity, simple operation, and rapid detection. The development of nanomaterials, antifouling coatings, and isothermal amplification technology has enabled a significant improvement in the performance of electrochemical biosensors, including sensitivity and specificity and sensor stabilities, etc. Nevertheless, to accomplish their application in clinical use, they require further improvement in several aspects, including sensor accuracy, miniaturization, and intelligence of instruments, and the assumption of long-term monitoring in vivo, which will provide a bright future for their diagnostic and prognostic clinical applications.

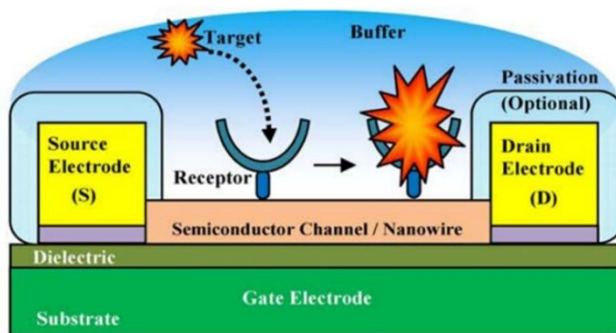

**Figure 12:** Experimental illustration of a nanoscale FET biosensor.<sup>144</sup>


**POINT-OF-CARE (POC) APPROACHES FOR HPV DETECTION: CURRENT STATUS**

**Screen-printed electrodes (SPE)** are usually used for measurements carried out for research in areas such as medicine, pharmacy, food industry, agriculture, environment, or national security.<sup>127</sup> Screen-printed electrodes can be fabricated, configured, and designed to be used in electrochemical applications for the detection and identification of drugs, pathogenic microorganisms, viruses, and protein biomarkers for diseases such as cancer, metabolic syndrome (MS) and for clinical analysis purposes in order to avoid human health problems. Moreover, they can be built as sensor arrays that allow the determination of multiple substances in parallel. Various studies that have been carried out using screen-printed electrodes and electrochemical analysis have shown that the material from which the working electrode (WE) exhibits a major role in the

modulation of the electrochemical response. Hence the functionalization and modification of the working electrode by different bodies or elements to detect the target analyte is of utmost importance in its fabrication. Screen-plated electrodes are named after the element from which the working electrode is made, thus there are carbon, gold, platinum, palladium, or other metals. The screen-printed carbon seems to be the electrode of choice for researchers when it comes to developing fast and cost-effective methods to detect or quantify disease-inducing agents. A typical screen-plated electrode can be connected to an amplifier – potentiostat and subjected to various electrochemical measurements. It contains a working electrode (WE), an auxiliary or counter electrode (CE) and reference electrode (RE). There are some with a 4-electrode variation which comprises a working electrode, working sense, auxiliary /counter electrode, and reference electrode.

Lately, research for the development of biosensors has exploded becoming a field of research for each type of biosensor, i.e., DNA (Deoxyribonucleic acid)-based sensors (genosensors), aptasensors, immunosensors, and enzymatic biosensors. In a recent review Mincu et al.<sup>146</sup> the authors reported that the aptamer-based sensors showed slightly better specificity and affinity for cancer-related biomarkers in comparison to antibodies-based sensors (immunosensors). In essence, screen-plated electrodes have come to the fore in the development of rapid in vitro diagnosis methods their functionalization and immobilization with molecules like proteins, antibodies, antigens, enzymes, oligonucleotides, etc in the development of these investigations. The early diagnosis of cervical cancer as a vital factor for its successful treatment cannot be overemphasized. A current report by Keyvani et al.<sup>147</sup> documented a novel integrated microfluidic electrochemical assay (IMEAC) that enables the detection of hr-HPV16-cDNA in

extracted plasma sample. The detection is achieved via graphene oxide (GO) modified screen-plated carbon electrode (SPCE) immobilized with cssDNA probe molecules that perceive the hr-HPV16 cDNA target (Figure 13). The concentration range of hr-HPV cDNA in the plasma of cervical cancer is 1099 copies per ml while the authors reported a limit of detection (LOD) of 0.48  $\mu\text{M}$  which is translated to  $\sim 10^9$  copies per ml. And though the LOD obtained does not cover the clinical range, it is the first time work on the detection of hr-HPV DNA in plasma has been reported. They also believe that the IMEAC can be potentially used in identifying other biomarkers of cervical cancer like hr-HPV18 cDNA from plasma by using suitable probe molecules, thus enabling multiplexed measurement. It is envisaged that IMEAC (after some modifications to enhance its detection potencies and specificity) will be as a point-of-care diagnostic device for screening cervical cancer in remote areas.

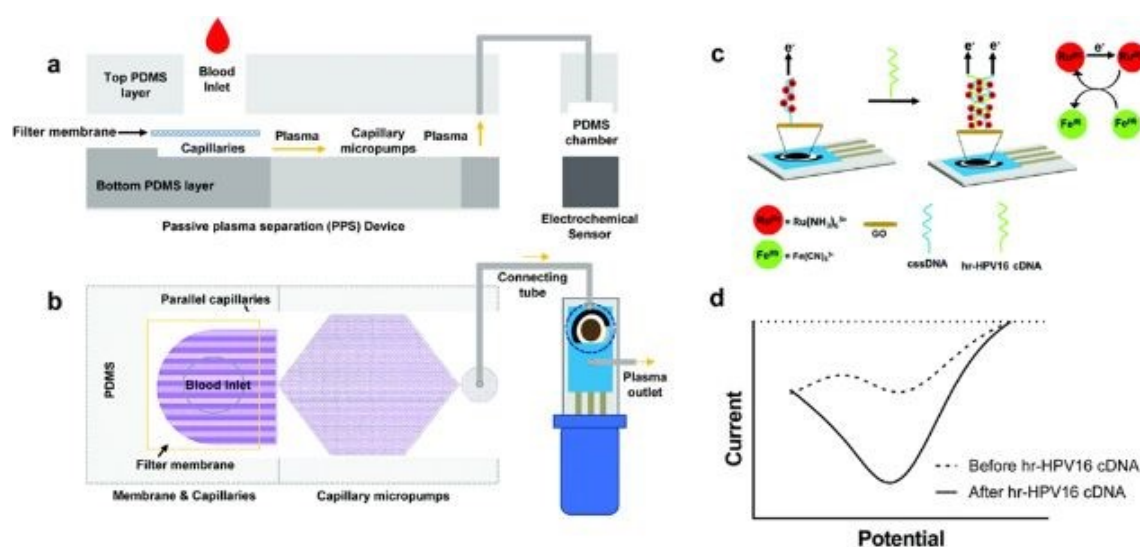

**Figure 13:** Overview and working mechanisms of IMEAC. Side view (a) and top view (b) of the IMEAC device that integrates two main modules: PPS for plasma isolation and an electrochemical biosensor. (c) Working principle of the electrochemical sensor for hr-HPV16 cDNA detection. (d) A sample graph extracted from IMEAC showing the presence of hr-HPV cDNA in the extracted plasma sample.<sup>147</sup>

Rawat et al.<sup>124</sup> developed a flexible electrochemical DNA biosensor for the detection of HPV-16. The biosensor was fabricated using carbon coated SPEs which was initially coated with reduced graphene oxide (rGO) followed by the probe DNA (PDNA) immobilization. The novel CSPE/rGO/DNA bio-nanohybrids possess a significant number of carboxyl groups for the efficient anchoring of HPV-16 PDNA. The sensor exhibited a LoD of  $\approx 2$  pM, was found to be selective solely to HPV-16 target DNA with a shelf life and response time of 1 month and  $\approx 15$  s. Bartosik et al.<sup>148</sup> presented a SPE electrode that was assembled by the means of streptavidin-modified magnetic beads and a DNA capture probe to detect HPV16 DNA by using a digoxigenin label. The detection range of this biosensor was 1 pM to around 1 nM. Jampa et al.<sup>149</sup> used a screen-printed electrode (SPE) immobilized with anthraquinone (AQ)-labeled pyrrolidinyl peptide nucleic acid (PNAs) for identifying HPV L1 gene down to 4 nM. A screen-printed gold electrode was used as an electrochemical resistive DNA biosensor. Espinosa et al.<sup>150</sup> to immobilize a DNA probe, complementary human papillomavirus type 16 (HPV-16) sequence. The presence

a complementary sequence was detected by the change in resistance when the ssDNA is transformed in dsDNA due to the hybridization event. The detection limit of 2.39 nM was obtained. The authors also boast of a very short detection time out -750  $\mu\text{s}$ , in the resistive HPV-16/DNA/Au ensemble biosensor which makes it a new fast technique compared to the traditional EIS applied to DNA biosensors.


### Paper-based PoC platforms

The attractiveness of Paper-based platforms in electrochemical sensing is because of their innate and interesting features which include their abundance, porosity, strong capillary action, disposability, lightness, flexibility, biocompatibility, eco-friendliness, and low cost.<sup>153,154,155</sup> Paper-based electrochemical (bio)sensors have been employed to determine target analytes in highly variable matrices—soils, exhaust gases, waters, industrial sewage, cellular extracted DNA, blood, plasma, serum, urine, sweat, exhaled breath, and pharmaceutical capsules.<sup>156-166</sup> Moreover, some of these (bio)devices made from paper-based substrates exhibit antifouling

properties that are highly pursued to ensure the proper functioning of the devices in real biological matrices. The introduction of Electrochemical paper-based analytical devices (ePADs) has further intensified and opened a myriad of research in this field.<sup>167</sup> It has launched a variety of fabrication procedures using different forms of paper materials like microfluidic PADs (μPAD).<sup>168,169,170</sup> Yakoh et al.<sup>171</sup> fabricated a 3D sequential fluid delivery platform on a microfluidic paper-based device (sePAD) which can store and transport reagents sequentially to the detection channel without the need for external power, thus eliminating multiple-step reagent manipulation inherent to complex bioassays. The device comprises two components, which are an origami folding paper (oPAD) and a movable reagent-stored pad (rPAD) with two

different configurations: the flow-through architecture, developed for continuous flow electrochemical measurements, such as chronoamperometry, and the stop-flow architecture, developed for non-convective electrochemical measurements, such as voltammetry. The 3D capillary-driven device served as an amperometric sensor for ascorbic acid determination; used for differential-pulse voltametric determination of serotonin and applied as an impedimetric immunosensor of α-fetoprotein detection.

Draz et al.<sup>172</sup> developed paper-plastic microchip (PPMC) comprising three-layer hybrid substrates prepared of a cellulose paper substrate assembled with a transparent plastic sheet by double-sided adhesive (DSA), as seen in **Figure 14**.

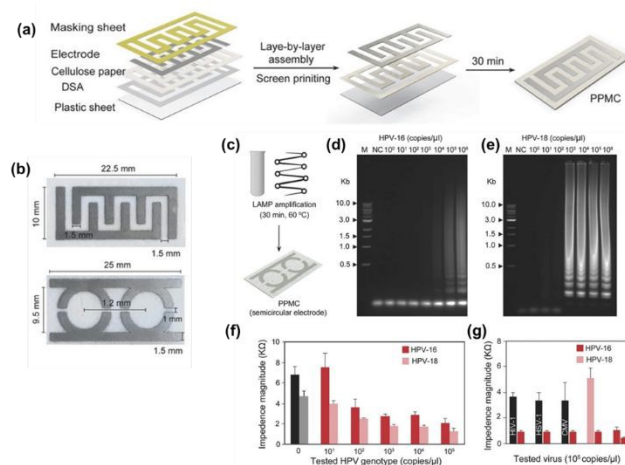

**Figure 14:** PPMC fabrication and characterization. (a) Fabrication of PPMC system using the screen-printing protocol coupled with layer-by-layer assembly. (b) Digital images of PPMC developed with interdigitated four-finger electrodes for single plex detection and two-semicircular electrodes for multiplex detection. HPV nucleic acid detection and genotyping using PPMC with semi-circular electrodes (c) Schematic presentation of the developed PPMC-based nucleic acid assay for HPV DNA detection. Loop-mediated isothermal amplification (LAMP) technique was used to amplify the target HPV DNA using a set of four specific primers for each tested genotype by independent reactions and the formed amplicons were loaded on PPMC for impedance measurements. (d) and (e) Gel electrophoresis of LAMP amplification products generated from different concentrations of HPV DNA template. LAMP reaction was performed using tenfold serial dilutions of HPV DNA template ( $1 \times 100$  copies per microliter to  $1 \times 10^6$  copies per microliter). M: 1-kb DNA ladder marker; NC: negative control (without target DNA template). (f) Impedance magnitude of LAMP amplicons prepared from different concentrations of target HPV templates at 8000 Hz and 1 V. For each concentration, the impedance magnitude was initially measured for LAMP amplicons of HPV-16 loaded on one of the testing zones and then for LAMP amplicons of HPV-18 loaded on the other testing zone. (g) Impedance magnitude of LAMP amplicons prepared from the target HPV-16 and nontarget viruses and genotype of human immunodeficiency virus-1 (HIV-1), herpes simplex virus-1 (HSV-1), and cytomegalovirus (CMV). Error bars represent the standard error of the mean calculated of at least three independent trials.<sup>172</sup>

The fabrication process of PPMC is simple and leverages the advantages of the well-known layer-by-layer assembly and screen printing protocols. The microchip with an upper surface made of cellulose paper and a lower back layer of plastic was adopted for electrical sensing of different targets, including liver and colon cancer biomarkers, and human papillomavirus (HPV). Coupled with loop-mediated isothermal amplification (LAMP), the developed PPMC electrodes were used for nucleic acid testing and genotyping of HPV. Two sets of primers, each comprising four specific primers, which are specific for two different genotypes of HPV-16 and HPV-18, were used for LAMP amplification. The formed LAMP amplicons in each reaction were simultaneously tested on PPMC designed with two detection zones (one was specified for HPV-16 and the other for HPV-18). The authors reported ladder-like amplicons, characteristic of LAMP was observed for both HPV-16 and HPV-18, confirming specific amplification of the target HPV genotype. The loading of LAMP amplicons to the surface of PPMC resulted in a significant

decrease in the impedance magnitudes measured at 8000 Hz and 1 V. The change in the impedance magnitude was inversely proportional to the tested concentration of the target HPV plasmid used in the samples of both HPV genotypes tested. Using this approach, the proposed PPMC can detect concentrations as low as  $10^2$  copies per microliter and  $10^3$  copies per microliter of HPV-16 and HPV-18, respectively.

Teengam, et al.<sup>121</sup>, built an ePAD-based peptide nucleic acid biosensor for selectively detecting HPV-16. It was developed using an anthraquinone-labeled pyrrolidiny peptide nucleic acid (acpcPNA) probe (AQ-PNA) and graphene-polyaniline (G-PANI). An inkjet printing technique was employed to prepare the paper-based G-PANI-modified working electrode. The paper-based electrochemical DNA biosensor was used to detect a synthetic 14-base oligonucleotide target with a sequence corresponding to human papillomavirus (HPV) type 16 DNA by measuring the electrochemical signal response of the AQ label using square-wave voltammetry






1 before and after hybridization. It was determined that the current  
2 signal significantly decreased after the addition of target DNA. This  
3 phenomenon is explained by the rigidity of PNA-DNA duplexes  
4 which obstructs the accessibility of electron transfer from the  
5 label to the electrode surface. Under optimal conditions, the  
6 detection limit of HPV type 16 DNA was found to be 2.3 nM with a  
7 linear range of 10–200 nM. The performance of this biosensor on real  
8 DNA samples was tested with the detection of PCR-amplified DNA  
9 samples from the SiHa cell line.

10 A comprehensive review on colorimetric paper-based sensors was  
11 done by Carneiro et al.<sup>173</sup> in which the authors set out to elucidate  
12 the application of paper as a substrate in sensor devices and the use  
13 of colorimetry for signal transduction and detection of cancer  
14 biomarkers. They surmised that improvements in the signal-to-noise  
15 amplification strategies have advanced and promoted the  
16 development of paper-based analytical devices (PAD) over the years  
17 that the use of novel materials like nanoparticles as labels has  
18 increased sensitivity and provided clear signals based on color  
19 change. They, however, stated that reports on real-world  
20 applications of PADs for colorimetric detection of biomarkers, such  
21 as cancer, are still very limited. Thus, more research is needed to  
22 identify and address the challenges of this technique which include  
23 high limits of detection, insufficient specificity, poor stability, the  
24 need for multiplexing, and subjective interpretation of the results.

### Smartphone-based platforms

View Article Online  
DOI: 10.1039/D4AY01921K

The new technological era has ushered in a wave of having everything either in miniature or converted to portable accessories. An example is combining conventional biosensing technologies with handy, portable, and easy-to-carry mobiles. With the knowledge of the extreme societal penetration of smartphones and their common presence, mobile-sensing approaches offer significant advantages over traditional platforms. Synergistic use of sensing technologies with mobile technology enables the development of powerful portable platforms for various applications. Smartphone capabilities include cameras, touchscreens, networking, computation, 3D sensing, audio, and motion, in addition to commercial wearable peripheral devices that can be leveraged for biomedical imaging. And through the user-centred design of custom hardware and software interfaces, these capabilities have the potential to enable portable, easy-to-use, point-of-care biomedical imaging systems. Hunt et al.<sup>174</sup> listed some smartphone-based imaging (SBI) systems which they categorized into four groups centred on their intended applications and clinical workflow: ex vivo diagnostic, in vivo diagnostic, monitoring, and treatment guidance. (Figure 15).

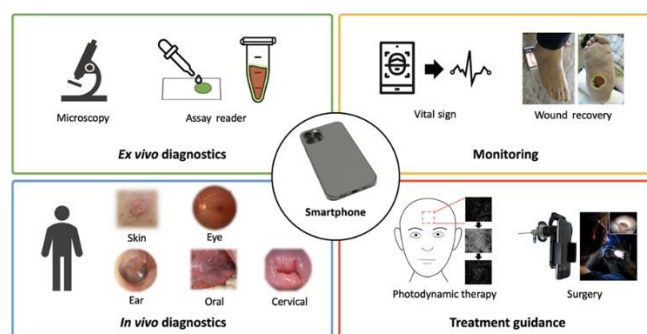

**Figure 15:** Smartphone-based imaging (SBI) for various biomedical imaging applications grouped into four clinical workflows.<sup>174</sup>

Naorungroj et al.<sup>175</sup> developed a smartphone-assisted paper-based colorimetric assay using pyrrolidiny peptide nucleic acid (acpcPNA) as a probe for the detection of HPV DNA. Dextrin-stabilized gold nanoparticles (d-AuNPs) were used as the colorimetric reagent. After the duplex formation between the acpcPNA probe and the HPV DNA target, the acpcPNA probe was depleted and the residual probe caused different degrees of d-AuNPs aggregation, resulting in a detectable color change. The different color change before and after the introduction of the DNA target as a function of the DNA concentration was quantified by analysing the colour intensity using the smartphone. The authors reported that under optimal experimental conditions, the colorimetric DNA sensor displayed a linear range for the detection of HPV DNA in the range of 1–1000 nM with a detection limit of 1 nM. It showed high stability for up to 60 days when stored at 4 °C with the percentage decrease of the signal being less than 10%. For real samples application, the developed sensor was successfully applied to detect PCR-amplified HPV DNA from cell line samples. To enhance their capabilities, a high-resolution microscope can be attached to a camera-enabled mobile phone, which enabled both bright-field and fluorescence imaging.<sup>176</sup> Prompt and reliable triaging of high-risk HPV cases could

help offset severe pathology bottlenecks in resource-limited regions and circumvent geographical and/or socioeconomic barriers to effective cervical cancer screening. Visual inspection with acetic acid (VIA) is adopted as a rapid, inexpensive alternative to standard cytology (Pap smears); however, it suffers from high rates of false-negative and false-positive results. This has triggered the application of the smartphone as an assisted accessory to the normal use of naked-eye visual inspection. In a recent study carried out among HPV-positive women living with HIV (WLWH) in Western Kenya, Mungo et al.<sup>179</sup> reported that digital images of the cervix were taken (WLWH of 25–49 years) using a smartphone by a nonphysician provider following visual inspection with acetic acid. These digital images were evaluated by three off-site colposcopists for quality and diagnostic utility and assigned a presumed diagnosis. Judging by the off-site expert colposcopists, the images were of good quality and had diagnostic utility. However, they observed low sensitivity for the diagnosis of CIN2+ from the cervical images compared with histopathology which if used for triage would result in substantial loss of opportunity for treatment of high-grade precancer in a high-risk population.

Open Access Article. Published on 23 December 2024. Downloaded on 16/20/25 5:53:11. This article is licensed under a Creative Commons Attribution 3.0 Unported Licence.



Champin et al.<sup>180</sup> conducted a systematic review to identify studies on the usefulness of the smartphone in detecting uterine cervical lesions. They reported that several studies reveal that digital images taken with a smartphone after a visual inspection with acetic acid (VIA) or Lugol's iodine (VILI) may be useful for detecting CIN. The smartphone images clicked after a VIA were found to be more sensitive than those following the VILI method or the VIA/VILI combination and naked-eye techniques in detecting uterine cervical lesions. Therefore, the authors surmised that smartphones could be useful in the early detection of uterine cervical lesions and could be an alternative to colposcopy in countries with limited health resources. However, they noted, its sensitivity and specificity are still limited. Dufeil et al.<sup>181</sup> set out to determine whether combined examination by the naked eye and digital VIA [D-VIA] and VILI [D-VILI] improves the detection of CIN2+ as compared to the conventional evaluation. The combination of both methods yielded a sensitivity of 92.3% and a specificity of 23.2%. Indeed, the combination of VIA/VILI and D-VIA/VILI seems to provide an increase in sensitivity with an acceptable decrease in specificity. Although the authors advised a replication of the study with a larger sample size would be necessary to draw definitive conclusions. Nonetheless, they are convinced that the digital cervical image is useful for the diagnosis of CIN2+ lesions as their study represents the best available evidence to date that suggests that D-VIA/VILI may potentially improve cervical cancer screening.


Recently, some authors reported on studies aimed to provide an evaluation of available data for smartphone use in low-resource settings in the context of D-VIA-based cervical cancer screenings between the years 2015 and 2021.<sup>182</sup> The available results to date show that the quality of D-VIA images is satisfactory and enables CIN1/CIN2+ diagnosis and that a smartphone is a promising tool for cervical cancer screening monitoring and for on- and off-site supervision, and training. The images obtained can be stored in a VIA image bank and used for training. Also, sharing real-time images with long-distance experts will improve the quality of work of healthcare providers. Although the evidence supports that D-VIA improves CIN2+ diagnostic performance, the use of smartphone applications is only considered a tool to minimize the subjectivity of the diagnosis. They further advised that a computer-assisted automated visual evaluation will be able to discriminate between normal and CIN and

will likely significantly improve diagnostic accuracies, as well as allow see-and-treat approaches. Thus, low LIMC healthcare providers should focus on the implementation and development of smartphone-based screening programs using D-VIA, as it is proven to be acceptable and inexpensive, and it aligns with the WHO's effort toward the elimination of cervical cancer in the twenty-first century.

## Conclusions and future outlooks

In this review, the advantages, and shortcomings of the traditional and emergent tools for screening and testing of HPV infections and cancer have been highlighted. To achieve the WHO's ambitious 2030 goal (i.e., every country ensuring that 70% of their women are screened using a high-performance test by the age of 35, and again by the age of 45) will require the adoption of two or more techniques based on nucleic acids and immunological techniques. Currently, the PCR-based methods dominate the clinical detection tools for HPV infection. However, some recent reports<sup>183,184</sup> the authors indicated that the application of immunology-based methods are "under reconsideration" as the probable precise strategies for accurate and sensitive diagnosis of HPV infection and cervical cancer. The reason for this emerging development is that PCR-based methods "can only be used to detect HPV DNA and HPV types and cannot be used to accurately predict HPV-positive cancers". Immunological methods based on antigens and antibodies are characterized by their high affinity, high specificity, and biocompatibility, thus important for the development of high-performance diagnostic tools for HPV infection and cervical cancer.

Interestingly, the reconsideration of immunological methods for accurate HPV detection bodes well for fast realization of clinically relevant electrochemical immunosensing devices for HPV infection. It is interesting in the sense that electrochemical immuno-/bio-sensing techniques are characterised by simplicity (do not require highly skilled personnel), low-cost compared to other methods, highly sensitive, highly specific, easily to be miniaturize (portability), fast (quick analytical results) and highly reproducible. As shown in **Figure 16**, three of the four traditional techniques for HPV detection (known for the low to moderate sensitivity and specificity) are already being reported in the literature but can be optimized to complement the other molecular biology-based methods.

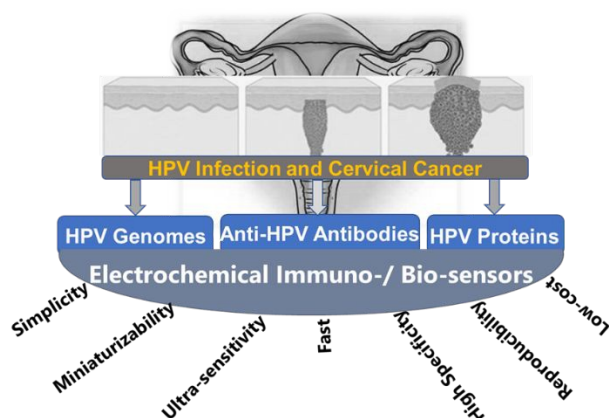


**Figure 16:** Schematic representation of the applicability of electrochemical methods for the detection of HPV infection and cancer through the detection of HPV genomes, Anti-HPV antibodies, and HPV proteins.

ARTICLE

View Article Online  
DOI: 10.1039/D4AY01921K

1 In our view, the effective screening of HPV infection in resource-limited countries will require multi-disciplinary activities as depicted in **Figure 17**. The access to digital camera is an important development in resource-limited societies that will positively impact on the effective screening of HPV infection. The patient's samples analysed with the appropriate portable point-of-care diagnostic device (powered by artificial intelligence for increased sensitivity) the results (data) are sent to the cloud server via a smart phone, results are passed on to the medical facility for informed decision making that will allow for appropriate medication and / or further treatment. Makower et al.<sup>185</sup> in a report had stated that to improve the chance of having a technology that could transfer from an academic concept to a diagnostic system, scientists may have to consider a new diagnostic tool which overcome an "actual" problem/diagnostic request, and the current solution to it should be inadequate/expensive. The authors further surmised that such diagnostic tools used for medical examination outside of medical labs (at home

without skilled operators) must be precise, be user-friendly for untrained people, and have little risk of user confusion or harm if performed incorrectly. The diagnostic systems should be able to relay the test results automatically and safely to cloud-based systems, with appropriate maintenance of privacy. The prevalence of HPV infections remains high especially in developing countries despite tremendous efforts for HPV treatment and prevention. Currently, Visual inspection with acetic acid (VIA) is adopted as a rapid, inexpensive alternative to standard cytology (Pap smear) is the main approach for the detection of early lesions of cervical cancer. The technique has however improved over the years, with the assistance of earlier cited technologies. In contrast, DNA testing for high-risk oncogenic HPV (subtypes 16 and 18) confers superior sensitivity (96-100%) and specificity (90-100%) along with greater clinical benefit when compared to cytology or VIA. This facilitates clinical counselling, follow-up examinations, thus improving treatment outcomes.

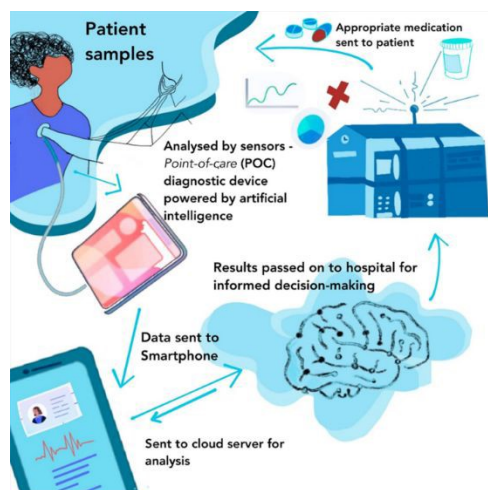

**Figure 17:** Schematic representation of the multi-disciplinary activities proposed for the prevention and control of HPV infection in the healthcare sector of resource-limited countries. The point-of-care diagnostic devices could be deployed for HPV infection and drug-monitoring, with dynamic spectrum broadband technology for an e-health that relies on secure data transmission from decentralized clinical benches (anywhere in the remote area) to the centralized laboratory, clinics, or hospitals.

43 Electrochemical immuno-/biosensors offer an inexpensive, sensitive,  
44 simple, rapid, and portable alternative for viral detection that  
45 improves POC testing in ways that conventional methods have  
46 failed.<sup>186</sup> These devices give access to early diagnosis of diseases  
47 resource-limited settings, helping the world fight diseases efficiently.  
48 They can also be operated using different analytes. Antibody-based  
49 systems are a viable option for HPV point-of-care diagnostics, which  
50 is demonstrated in their longstanding popularity.<sup>187</sup> Some antibody-  
51 based diagnostic tools have made it from the laboratory to the  
52 consumer stage. An example is the OncoE6™ from Arbor Vita which  
53 is a lateral flow cervical cancer test device that detects the presence  
54 of E6 onco-proteins from high-risk types of human papilloma virus  
55 (HPV) types 16 and 18. However, the test takes 2.5 h, which is a  
56 significant length of time for a POC test.

The introduction of lectins and aptamers are contributing to POC testing due to their capacity for glycoprofiling. Jin et al.<sup>188</sup> used an enzyme-linked lectin assay (ELLA) for detecting cervical intraepithelial neoplasia I (CIN I) and cervical cancer using serum immunoglobulins (Ig). The lectin-based assays such as ELLAs were found to have similar specificity and sensitivity to those seen in antibody-based ELISAs along with their ability to distinguish between glycosylation patterns. On the other hand, the authors reported that ELLAs were superior in discriminating CIN I and cervical cancerous cells from healthy cells while ELISAs were better able to differentiate between CIN I and cervical cancerous cells. Non-invasive biomarkers have come up as could be "game-changers" in the early detection of cervical cancer. Some urinary proteins are being identified and used as biomarkers in early cervical cancer screening. This has also opened an avenue to self-sampling

Open Access Article. Published on 23 December 2024. Downloaded on 16/12/2024 11:52:53 PM. This article is licensed under a Creative Commons Attribution 3.0 Unported Licence.



1 methods for early cervical cancer detection.<sup>189,190,191</sup> Basak et al.<sup>24</sup>  
 2 identified a protein biomarker antigen (NCB-Ag) prote<sup>25</sup>  
 3 phosphatase-1-gamma-2 (PP1γ2) specific to cervical cancer<sup>26</sup>  
 4 expressed in the urine sample. The antibody (Ab) specific to the NCB<sup>27</sup>  
 5 Ag is attached to plasmonic Au NPs (≈ 5-20 nm) through a DTSP (3,<sup>28</sup>  
 6 dithiodipropionic acid di (*n*-hydroxysuccinimide ester) linker to for<sup>29</sup>  
 7 a composite Ab-DTSP-Au-NP. A localized surface plasmon resonanc<sup>30</sup>  
 8 (LSPR)-based immunosensing method was used for the qualitativ<sup>31</sup>  
 9 reliable, and specific detection of the biomarker; thus, the Ab-DTS<sup>32</sup>  
 10 Au-NP composite undergoes a plasmonic shift after the interactio<sup>33</sup>  
 11 with NCB-Ag in urine samples.<sup>34</sup>  
 12 In a very recent advancement, Chen et al.<sup>191</sup> developed a novel<sup>35</sup>  
 13 photothermal triggered multi signal readout POC testing using<sup>36</sup>  
 14 multifunctional vagina swab for HPV 17 E6 protein determinatio<sup>37</sup>  
 15 The quantitative detection of target analyte was performed by usin<sup>38</sup>  
 16 a portable fluorescence spectrometer and an inexpensive pressu<sup>39</sup>  
 17 meter in only 1 min with high sensitivity and accuracy. The composi<sup>40</sup>  
 18 probe SiC-CS@Ag (silicon decorated nanoparticles on chitosan-C<sup>41</sup>  
 19 triggered sensitive fluorescent quenching on a flexible fluorescenc<sup>42</sup>  
 20 temperature indicator (FLTI) and a remarkable pressure variation<sup>43</sup>  
 21 pressure device under laser radiation. This bioassay realized sensitiv<sup>44</sup>  
 22 target detection in the linear ranger from 10<sup>-6</sup> ng/mL to 1 ng/mL with<sup>45</sup>  
 23 detection limits of 1.60 × 10<sup>-6</sup> ng/mL.<sup>46</sup>

## 47 Author contributions

48 Omobosedede O. Fashedemi, investigation, writing-original draft<sup>47</sup>  
 49 figure drawing, Okoroike C. Ozoemena, investigation, visualization<sup>48</sup>  
 50 review, editing Siwaphiwe Peteni, investigation, visualization review<sup>49</sup>  
 51 editing, Aderemi B. Haruna, reviewing, editing, investigation<sup>50</sup>  
 52 Leshweni J. Shai, Aicheng Chen, Frankie Rawson, Maggie<sup>51</sup>  
 53 Cruickshank, David Grant, Oluwafunmilola Ola, reviewing<sup>52</sup>  
 54 conceptualization, supervision, and Kenneth I. Ozoemer<sup>53</sup>  
 55 conceptualization, reviewing, supervision<sup>54</sup>

## 56 Conflicts of interest

57 There are no conflicts to declare.<sup>55</sup>

## 58 Data availability

59 All the data is presented on this review paper.<sup>56</sup>

## 60 Acknowledgements

61 The authors are grateful for funding from Cancer Research UK<sup>57</sup>  
 62 (EDDPMA-May21\100042), EPSRC (EP/Y003225/1) and the South<sup>58</sup>  
 63 Africa's National Research Foundation (NRF) through the SARC<sup>59</sup>  
 64 Chair in Materials Electrochemistry and Energy Technologies (MEET<sup>60</sup>  
 65 (UID No.132739).<sup>61</sup>

Machine learning and artificial intelligence, though still expensive  
 cannot be left out in POC cervical cancer diagnostics.<sup>NEW ARTICLE ONLINE</sup>  
 Pathania et al.<sup>192</sup> developed an Artificial Intelligence Monitoring for HPV (AIM-  
 HPV), that integrates low and high-tech solutions for DNA-based and  
 POC cervical cancer screening. A disposable DNA extraction kit based  
 on manual syringe operations was fabricated. This kit is a DNA-  
 focused digital micro-holography platform monitoring for point-of-  
 care HPV screening., with automated readouts driven by customized  
 deep-learning algorithms. It incorporates microbeads designed to  
 bind HPV 16 or 18 DNA targets and form microbead dimers. The  
 authors reported the HPV DNA assay showed excellent sensitivity  
 (down to a single cell) and specificity (100% concordance) in  
 detecting HPV 16 and 18 DNA from cell lines. The deep learning  
 approach was 120-fold faster than the traditional reconstruction  
 method and completed the analysis in < 2 min using a single central  
 processing unit (CPU).

This review has attempted to capture the different point-of-care  
 approaches for HPV detection, the challenges involved, and new  
 advances and technologies to mitigate these challenges. As  
 mentioned earlier some of these innovations can serve both  
 diagnostic and prognostic purposes in HPV screening which can be  
 integrated into primary health settings in LMICs as screen-and-treat  
 models.

## Notes and references

- 1) E. Peeters, K. Cornet, H. Cammu, V. Verhoeven, D. Devroey, M. Arbyn, *Papillomavirus Res*, **2020**, *9*, 100194.
- 2) S. V. Graham, *Future Microbiol.*, **2010**, *5*, 1493-506.
- 3) L.Yu, V. Majerciak, Z. M. Zheng, *Int. J. Mol. Sci.*, **2022**, *23*, 4943
- 4) Arumugam, M. Ranajit Kumar, G. Suvankar Ghora, J. Saikat Kumar, *J. Electrochem. Soc*, **2024**, *171*, 027519
- 5) L. Pan, B. Li, J. Chen, H. Zhang, X. Wang, J. Shou, D. Yang, X. Yan, *Front Chem*, **2021**, *9*, 798727.
- 6) S. Rubina, C.M. Krishna, *J Cancer Res Ther* **2015**, *11*, 10-17.
- 7) C.W.E. Redman, V. Kesic, M.E. Cruickshank, M. Gultekin, X. Carcopino, M. Castro Sanchez, M. Grigore, M. Jakobsson, V. Kupperts, A. Pedro, O. Reich, S. Leeson, U. Tabuica, J. Zodzika, A. Ciavattini, R. Jach, M. Katsyuba, R. Koiss, P. Martin-Hirsch, W.A. Tjalma, P. Nieminen, *Eur J Obstet Gynecol Reprod Biol*, **2021**, *256*, 57-62.
- 8) B. Nedjai, C. Reuter, A. Ahmad, R. Banwait, R. Warman, J. Carton, S. Boer, J. Cuzick, A. T. Lorincz, *Int J Cancer.*, **2018**, *143*, 1720-1730],
- 9) B. Gardella, M. Dominoni, M. F. Pasquali, C. Melito, G. Fiandrino, S. Cesari, M. La Verde, A. Spinillo, *Vaccines*, **2023**, *11*, 284.
- 10) L. Galati, S. Chiocca, D. Duca, M. Tagliabue, C. Simoens, T. Gheit, M. Arbyn, M. Tommasino, *Tumour Virus Res.*, **2022**, *14*, 200245.
- 11) M. Preti, J. C. Rotondo, D. Holzinger, L. Micheletti, N. Gallio, S. McKay-Chopin, C. Carreira, S.S. Privitera, R. Watanabe, R. Ridder, M. Pawlita, C. Benedetto, M. Tommasino, T. Gheit, *Infect Agent Cancer*, **2020**, *15*, 20.
- 12) L. Pekarek, M. A. Ortega, O. Fraile-Martinez, C. García-Montero, C. Casanova, M. A. Saez, N. García-Honduvilla, M. Alvarez-Mon, J. Buján, V. Diez-Nicolas, J.F. Burgos, V. Gomez Dos Santos, *J Pers Med.*, **2022**, *12*, 1364
- 13) A. L. Hernandez, J.F. Hilton, C. S. Weatherly, et al., *J Acquir Immune Defic Syndr*, **2024**, *96*, 439-446
- 14) R. Ravindran, S. Cotton, M. Cruickshank, *Cytopathology*, **2020**, *31*, 47-52.



1 15) G. Murewanhema, E. Moyo, M. Dzobo, R. 67  
 2 Mandishora-Dube, T. Dzinamarira, Vaccine: X, 2024, 268  
 3 100549 69  
 4 16) J. M. Kutz, P. Rausche, T. Gheit, et al., BMC Pub 70  
 5 Health, 2023, 23, 974 71  
 6 17) T.B.R. Freeman-Wang, M.E. Cruickshank, H.C. Kitchener, 72  
 7 Scientific Impact Paper, 2016, 7, 1-9. 73  
 8 18) L. Denny, L. Kuhn, M. De Souza, A. E. Pollack, W. Dupre 74  
 9 T. C. Wright, Jr., JAMA, 2005, 294, 2173-2181. 75  
 10 19) S. Sayed, M. Chung, M. Temmermans, Lancet Gl 76  
 11 Health 2020, 8, e171-e172. 77  
 12 20) M.L. Wilson, K.A. Fleming, M.A. Kutu, L.M. Looi, N. Laga 78  
 13 K. Ru, Lancet, 2018, 391, 1927-1938. 79  
 14 21) A.D. Shrestha, D. Neupane, P. Vedsted, P. Kallestru 80  
 15 Asian Pac J Cancer Prev, 2018, 19, 319-324. 81  
 16 22) A.Goel, G. Gandhi, S. Batra, S. Bhambhani, V. Zutshi, 82  
 17 Sachdeva, Int J Gynaecol Obstet 2005, 88, 25-30. 83  
 18 23) R. L. Siegel, K.D. Miller, A. Jemal, 2019. CA Cancer J Clin 84  
 19 2019, 69, 7-34. 85  
 20 24) B. Prabhakar, P. Shende, S. Augustine, Biom 86  
 21 Pharmacother, 2018, 106, 1586-1599. 87  
 22 25) Z. Altintas, I. Tothill, Sensors and Actuators B: Chem 88  
 23 2013, 188, 988-998. 89  
 24 26) S. Mittal, H. Kaur, N. Gautam, A.K. Mantha, Bioproc 90  
 25 Bioelectron 2017, 88, 217-231. 91  
 26 27) C. Lasser, S.E. O'Neil, G.V. Shelke, C. Sihlbom, S 92  
 27 Hansson, Y.S. Gho, B. Lundback, J. Lotvall, J Transl Med 93  
 28 2016, 14, 181. 94  
 29 28) L. Gonzalez-Calero, M. Martin-Lorenzo, G. Alvarez 95  
 30 Llamas, Front Immunol, 2014, 5, 465. 96  
 31 29) R. Kishore, V.N.S. Garikipati, A. Gumpert, J Cardiovasc 97  
 32 Transl Res, 2016, 9, 169-175. 98  
 33 30) J. Howitt, A.F. Hill, J Biol Chem, 2016, 291, 26589-26599 99  
 34 31) M. Record, M. Poirot, S. Silvente-Poirot, Biochim Biophys 100  
 35 2014, 96, 67-74. 101  
 36 32) K.Z. Salem, M. Moschetta, A. Sacco, L. Imberti, G. Rossi, 102  
 37 I. M. Ghobrial, S. Manier, A.M. Roccaro, Methods Mol Biol, 2016, 1464, 25-34. 103  
 38 33) S. Sayed, W. Cherniak, M. Lawler, S.Y. Tan, W. El Saadani, 104  
 39 N. Wolf, S. Silkensen, N. Brand, L.M. Looi, S.A. Pai, et al., 105  
 40 Lancet, 2018, 391, 1939-1952. 106  
 41 34) L.P. Andre´, A.L. de Abreu, R.P. Souza, M.C. da Silva, M.C. 107  
 42 Uchimura, R.L. Zanko, E.C. Ferreira, M.C. Tognim, M.F. 108  
 43 Teixeira, F. Gimenes, M.E. Consolaro. Am. J. Trop. Med. Hyg. 109  
 44 2012, 87, 1149-1151. 110  
 45 35) L.L. Villa , L. Denny, Int J Gynaecol Obstet., 2006, 94, 111  
 46 571-580 . 112  
 47 36) J. Choi, C. Kim, H.S. Lee, Y.J. Choi, H.Y. Kim, J. Lee, J. 113  
 48 Chang, A. Kim , J Pathol Transl Med., 2016, 50, 442-450 114  
 49 37) A. Qvick, E. Andersson, A. Oldaeus Almerén, M. Waenerlund, 115  
 50 B. Stenmark, C. Karlsson, M. G. Karlsson, G. Helenius, Mol Diagn Ther., 2024, 28, 835-845. 116  
 51 38) G. Lillsunde Larsson, G. Helenius, Cell Oncol (Dordr), 2017, 40, 521-527. 117  
 52 39) Lv, Y. Zhao, Y. Song, M. Ji, Y. Zhou, BMC Cancer, 2021, 23,1022. 118  
 53 40) M. Schiff, P.E. Castle, J. Jeronimo, A.C. Rodriguez, J. Wacholder, The Lancet, 2007, 370, 890-907. 119  
 54 41) P.A. Cohen, A. Jhingran , A. Oaknin, L. Denny, The Lancet, 2019, 393, 169-182. 120  
 55 42) A. B. Moscicki, S. Farhat, J. Xu, The Journal of Infectious Diseases, 2004, 190, 37-45. 121  
 56 43) M. Afzal, I. Manzoor, O. P. Kuipers, J Vis Exp, 2015, 98, 1-9. 122  
 57 44) E. J. Blom, D. W. Blossman, S. A. van Hijum, R. Breitling, L. Tijmsma, R. Silvis, J.B. Roerdink, O. P. Kuipers, BMC Bioinformatics, 2007, 23, 1161-1163. 123  
 58 45) E. J. Blom, S. A. van Hijum, K. J. Hofstede, R. Silvis, J. B. Roerdink, O. P. Kuipers, BMC Bioinformatics, 2008, 9, 535. 124  
 59 46) E.J. Blom, R. Breitling, K.J. Hofstede, J.B. Roerdink, S.A. van Hijum, O.P. Kuipers, BMC Genomics 2008, 9, 495. 125  
 60 47) A. de Jong, H. Pietersma, M. Cordes, O.P. Kuipers, J. Kok, BMC Genomics, 2012, 13, 10. 126  
 61 48) L. Gogianu, M.C. Popescu, B.S. Vasile, I. Mihalache, E. M. Anghel, C.M. Damian, A. Salceanu, A. Boldeiu, E. Constantin, A. Radoi, et al., Appl. Surf. Sci., 2023, 636, 157878 127  
 62 49) S. Varesano, A. Pulliero, E. Martorana, G. Pizzino, G. Raciti, S. Coco, V.G. Vellone, A. Izzotti, J Pers Med, 2023, 13, 531. 128  
 63 50) Z. Q. Toh, L. He, C. Chen, A. Huang, F. M. Russell, S. M. Garland, R. Reyburn, T. Ratu, E. Tuivaga, I. H. Frazer, E. K. Mulholland, P. V. Licciardi, Front. Immunol., 2020, 11, 1-9. 129  
 64 51) R. Wang, Y. Wang, Int J Mol Sci, 2021, 22, 1206. 130  
 65 52) J.G. Kelly, J. Trevisan, A.D. Scott, P.L. Carmichael, H.M. Pollock, P.L. Martin-Hirsch, F.L. Martin, J Proteome Res, 2011, 10, 1437-1448. 131  
 66 53) T. Lilo, C. L.M. Morais, C. Shenton, A. Ray, N. Gurusinghe, Photodiagnosis Photodyn Ther, 2022, 38, 102785. 132  
 67 54) D. Finlayson, C. Rinaldi, M.J. Baker, Anal Chem, 2019, 91, 12117-12128. 133  
 68 55) B.R. Wood, L. Chiriboga, H. Yee, M.A. Quinn, D. McNaughton, M. Diem, Gynecol Oncol., 2004, 93, 59-68. 134  
 69 56) Y. Ma, F. Liang, M. Zhu, C. Chen, C. Chen, X. Lv, Photodiagnosis Photodyn Ther, 2022, 39, 103023. 135  
 70 57) M.R. Viana, I.M. Melo, N. J. Batista, L. J. Raniero, R.D. Canevari, Research, Society and Development, 2022, 11. 136  
 71 58) M.R. Pereira Viana, I. Martins Alves Melo, B. Pupin, L. J. Raniero, R. de Azevedo Canevari, Photodiagnosis Photodyn Ther, 2020, 29, 101592. 137  
 72 59) A. C. O. Neves, P.P. Silva, C. L. M. Morais, C.G. Miranda, J. C. O. Crispim, K. M. G. Lima, RSC Advances, 2016, 6, 99648-99655. 138  
 73 60) H. Mo, L. Yang, G. Wu, X. Zheng, J. Wang, L. Yin, X. Lv, Optik, 2020, 206, 164292. 139  
 74 61) T. Rymysza, E.A. Ribeiro, L. F. D. C. E. S. de Carvalho, T. Bhattacharjee, R. de Azevedo Canevari, Spectrochim Acta A Mol Biomol Spectrosc, 2018, 196, 238-246. 140  
 75 62) F. Le Naour, C. Sandt, C. Peng, N. Trcera, F. Chiappini, A. M. Flank, C. Guettier, P. Dumas, Anal Chem, 2012, 84, 10260-10266. 141  
 76 63) A. C. Talari, M.G. Martinez, Z. Movasaghi, S. Rehman, I. U. Rehman, Applied Spectroscopy Reviews, 2016, 52, 456-506. 142  
 77 64) I. R. Ramos, A. Malkin, F.M. Lyng, BioMed Res Int, 2015, 2015, 1-9. 143  
 78 65) M. S. Silva-López, C. A. Ilizaliturri Hernández, H. R. Navarro Contreras, A. G. Rodríguez Vázquez, A. Ortiz-Dosal, E. S. Kolosovas-Machuca, Appl. Sci., 2022, 12, 2419. 144  
 79 66) C. Chen, J. Wang, C. Chen, J. Tang, X. Lv, C. Ma, Optik, 2020, 210, 164514 145  
 80 67) X. Zheng, J. Wang, L. Yin, B. Luo, X. Lv, G. Wu, Laser Phys. Lett., 2020, 17, 115601. 146  
 81 68) D. Traynor, C.M. Martin, C. White, S. Reynolds, T. D'Arcy, J. J. O'Leary, F. M. Lyng, Cancers (Basel), 2021, 13, 2008. 147  
 82 69) K. Sitarz, K. Czamara, J. Bialecka, M. Klimek, B. Zawilinska, S. Szostek, A. Kaczor, Int J Mol Sci, 2020, 21, 2667. 148  
 83 70) K. Aljakouch, Z. Hilal, I. Daho, M. Schuler, S. D. Krauss, H. K. Yosef, J. Dierks, A. Mosig, K. Gerwert, S. F. El-Mashtoly, Anal Chem, 2019, 91, 13900-13906. 149

Analytical Methods Accepted Manuscript

- 1  
2  
3 1 71) L. Dan, Z. Li, Y. Gu, S. Ge, Y. Mao, Y. Gu, X. Cao, *Materials* **2022**, *15*, 1331-1343. 67  
4 2 72) J. Wang, C. X. Zheng, C. L. Ma, X. X. Zheng, X. Y. Lv, G. Lv, J. Tang, G. H. Wu, *Lasers Med Sci.*, **2021**, *36*, 1857-1864. 68  
5 3 73) P. R. Jess, D. D. Smith, M. Mazilu, K. Dholakia, A. Riches, C. S. Herrington, *Int'l J Cancer*, **2007**, *121*, 2723-2728. 69  
6 4 74) C. F. Ning, Y. F. Tian, W. Zhou, B. C. Yin, B. C. Ye, *Analyst*, **2019**, *144*, 2929-2935. 70  
7 5 75) S. Bu, X. Liu, Z. Wang, H. Wei, S. Yu, Z. Li, Z. Hao, W. Li, J. Wan, *Sensors and Actuators B: Chemical*, **2021**, *347*, 130630. 71  
8 6 76) B. Fang, Z. Jia, C. Liu, K. Tu, M. Zhang, L. Zhang, *Talanta*, **2022**, *249*, 123657. 72  
9 7 77) J. Zhang, C. Song, Y. Zhu, H. Gan, X. Fang, Q. Peng, Xiong, C. Dong, C. Han, L. Wang, *Biosens Bioelectron*, **2022**, *219*, 114836. 73  
10 8 78) K. Khambhati, G. Bhattacharjee, V. Singh, *J Cell Biochem*, **2019**, *120*, 2721-2725. 74  
11 9 79) L. Liu, J. J. Duan, X. Y. Wei, H. Hu, Y. B. Wang, P. P. Jia, S. Pei, *Sci Total Environ*, **2022**, *838*, 156048. 75  
12 10 80) P. Puig-Serra, M. C. Casado-Rosas, M. Martinez-Lage, Olalla-Sastre, A. Alonso-Yanez, R. Torres-Ruiz, Rodriguez-Perales, *S Int J Mol Sci* **2022**, *23*, 1757. 76  
13 11 81) D. G. Sashital, *Genome Med*, **2018**, *10*, 32. 77  
14 12 82) Y. Tian, T. Liu, C. Liu, Q. Xu, Q. Liu, *Microchemical Journal*, **2022**, *174*, 107036. 78  
15 13 83) X. Wang, X. Shang, X. Huang, *Emerg Microbes Infect*, **2020**, *9*, 1682-1691. 79  
16 14 84) Y. Li, F. Meng, C. Sui, Y. Wang, D. Cheng, *J Cell Commun Signal* **2022**, *17*, 627-638. 80  
17 15 85) L. Zhou, R. Peng, R. Zhang, J. Li, *J Cell Mol Med*, **2019**, *22*, 5807-5815. 81  
18 16 86) Z. Wang, W. Cui, *View*, **2020**, *1*, 1-22. 82  
19 17 87) A. Ghouneimy, Z. Ali, R. Aman, W. Jiang, M. Aouida, Mahfouz, *ACS Synth. Biol*, **2024**, *13*, 837-850. 83  
20 18 88) A. A. Aljabali, M. El-Tanani, M. M. Tambuwala, *J Deliv Sci and Technol*, **2024**, *92*, 105338. 84  
21 19 89) C. Gao, P. Wu, L. Yu. et al., *Cancer Gene Ther*, **2022**, *29*, 466-474. 85  
22 20 90) J. Zhuang, Z. Zhao, K. Lian, L. Yin, J. Wang, S. Man, G. L. Ma, *Biosens Bioelectron*, **2022**, *207*, 114167. 86  
23 21 91) J. Liang, P. Teng, W. Xiao, G. He, Q. Song, Y. Zhang, Peng, G. Li, L. Hu, D. Cao, Y. Tang, *J Nanobiotechnology*, **2021**, *19*, 273. 87  
24 22 92) J. Liu, J. Chen, D. Wu, M. Huang, J. Chen, R. Pan, Y. G. Li, *Anal Chem*, **2021**, *93*, 10167-10174. 88  
25 23 93) Y. Du, S. Ji, Q. Dong, J. Wang, D. Han, Z. Gao, *Anal Chim Acta*, **2023**, *1245*, 340864. 89  
26 24 94) J. H. Choi, M. Shin, L. Yang, B. Conley, J. Yoon, S. N. Lee, K. B. Lee, J. W. Choi, *ACS Nano*, **2021**, *15*, 13475-13481. 90  
27 25 95) A. Su, Y. Liu, X. Cao, W. Xu, C. Liang, S. Xu, *Sensors Actuators B: Chemical*, **2022**, *369*, 132295. 91  
28 26 96) R. Shaikh, A. Daniel, F. M. Lyng, *Molecules*, **2023**, *28*, 2502. 92  
29 27 97) H. Wang, A. Su, J. Chang, X. Liu, C. Liang, S. Xu, *Sensors & Diagnostics* **2023**, *2*, 792-805. 93  
30 28 98) A. Su, Y. Liu, X. Cao, J. Zhao, W. Xu, C. Liang, P. Li, S. Anal Chem, **2023**, *95*, 5927-5936. 94  
31 29 99) D. Paul, A. Kumar, A. Gajbhiye, M. K. Santra, R. Srikanth, *Biomed Res Int*, **2013**, *2013*, 783131. 95  
32 30 100) L. D. Bertzbach, B. B. Kaufer, A. Karger, *Adv Virus Res*, **2021**, *109*, 31-62. 96  
33 31 101) K. Schwamborn, R. C. Krieg, S. Uhlig, H. Ikenberg, Wellmann, *Int J Mol Med*, **2011**, *27*, 417-421. 97  
34 32 102) F. Godoy-Vitorino, G. Ortiz-Morales, J. Romaguera, M. Sanchez, M. Martinez-Ferrer, N. Chorna, *PLoS One*, **2018**, *13*. 98  
35 33 103) X. W. Zhang, Q. H. Li, Z. D. Xu, J. J. Dou, *RSC Adv* **2020**, *10*, 3092-3104. 99  
36 34 104) F. Cui, Z. Zhou, H. S. Zhou, *J. The Electrochem. Soc.*, **2020**, *167*, 037525. 100  
37 35 105) S. Bulck, J. Berkhof, N. W. Bulkman, G. D. Zielinski, L. Rozendaal, F. J. van Kemenade, P. J. Snijders, C. J. Meijer, *Br J Cancer*, **2006**, *94*, 171-175. 101  
38 36 106) K. Mahato, A. Kumar, P.K. Maurya, P. Chandra, *Biosens Bioelectron* **2018**, *100*, 411-428. 102  
39 37 107) L. Jing, C. Xie, Q. Li, M. Yang, S. Li, H. Li, F. Xia, *Anal Chem*, **2022**, *94*, 269-296. 103  
40 38 108) G. Yang, Z. Xiao, C. Tang, Y. Deng, H. Huang, Z. He, *Biosens Bioelectron*, **2019**, *141*, 111416. 104  
41 39 109) S. Van Keer M. Willhauck-Flekestein., J. Pattyna, J. Butt, W. A. A. Tjalma, X. Van Ostade, N. Hens, P. Van Damme, T. Waterboer, A. Vorsters, *J Clin Virol.*, **2019**, *117*, 11-18. 105  
42 40 110) O. C. Ozoemena, T. Maphumulo, J. L. Shai, K. I. Ozoemena, *ACS Omega*, **2020**, *5*, 5762-5771. 106  
43 41 111) M. Freitas, H. P. A. Nouws, C. Delerue-Matos, *Electroanalysis*, **2018**, *30*, 1584-1603. 107  
44 42 112) D. Yang, Y. Shi, Y. Tang, H. Yin, Y. Guo, S. Wen, B. Wang, C. An, Y. Wu, W. Gao, *J Cancer*, **2019**, *10*, 4455-4462. 108  
45 43 113) S. Damiati, B. Schuster, *Sensors*, **2020**, *20*, 1721. 109  
46 44 114) L. Farzin, M. R. Shamsipur, *J Pharm Biomed Anal*, **2018**, *147*, 185-210. 110  
47 45 115) A. Sinha, Dhanjai, S. M. Mugo, H. Zhao, J. Chen, R. Jain, In *Advanced Biosensors for Health Care Applications*, **2019**, 147-169. 111  
48 46 116) Y. M. Park, S. J. Kim, K. Kim, Y. D. Han, S. S. Yang, H. C. Yoon, *Sensors and Actuators B: Chemical*, **2013**, *186*, 571-579. 112  
49 47 117) P. S. Sfragan, G. Moro, F. Polo, I. Palchetti, *Biosensors (Basel)* **2021**, *11*, 246. 113  
50 48 118) X. Hai, Y. Li, C. Zhu, W. Song, J. Cao, S. Bi, *TrAC Trends in Analytical Chemistry*, **2020**, *133*, 116098. 114  
51 49 119) E. Rasouli, W. J. Basirun, M. R. Johan, M. Rezayi, M. R. Mahmoudian, D. P. Poenar, *Sensing and Bio-Sensing Research*, **2023**, *40*, 100562. 115  
52 50 120) I. Irkham, A. U. Ibrahim, P. C. Pwavodi, F. Al-Turjman, Y. W. Hartati, *Sensors*, **2023**, *23*, 2240. 116  
53 51 121) P. Teengam, W. Siangproh, A. Tuantranont, C. S. Henry, T. Vilaivan, O. Chailapakul, *Anal Chim Acta*, **2017**, *952*, 32-40. 117  
54 52 122) S. Pareek, U. Jain, M. Bharadwaj, K. Saxena, S. Roy, N. Chauhan, *Anal Biochem* **2023**, *663*, 115015. 118  
55 53 123) C. Wang, Q. Yan, H. B. Liu, X. H. Zhou, S. J. Xiao, *Langmuir*, **2011**, *27* (19), 12058-12068. 119  
56 54 124) R. Rawat, S. Roy, T. Goswami, A. Mathur, *Diagnostics*, **2022**, *12*, 2087. 120  
57 55 125) H. H. Kim, H. J. Jeon, H. K. Cho, J. H. Cheong, H. S. Moon, J. S. Go, *Sensors and Actuators B: Chemical*, **2015**, *221*, 1372-1383. 121  
58 56 126) S. Peteni, O. C. Ozoemena, T. Khawula, A. B. Haruna, F. J. Rawson, L. J. Shai, O. Ola, K. I. Ozoemena, *ACS Sens*, **2023**, *8*, 2761-2770. 122  
59 57 127) O. C. Ozoemena, T. J. Ehirim, T. Khawula, K. Makgopa, L. J. Shai, K. I. Ozoemena, *Electrocatalysis*, **2021**, *12*, 595-604. 123  
60 58 128) O. C. Ozoemena, N. S. Mathebula, T. J. Ehirim, T. Maphumulo, G. M. Valikpe, J. L. Shai, K. I. Ozoemena, *Electrochimica Acta*, **2020**, *356*. 124  
61 59 129) H. Asadi, R. P. Ramasamy, *J. Electrochem. Soc.*, **2020**, *167*, 167523. 125

1 130) A. Wang, Y. Zhou, Y. Chen, J. Zhou, X. You, H. Liu, Y. Li, P. Ding, Y. Qi, C. Liang, X. Zhu, Y. Zhang, E. Liu, G. Zhang, *Anal Biochem*, **2023**, 660, 114953. 71

2 131) T. J. Ehirim, O. C. Ozoemena, P. V. Mwonga, A. Haruna, T. P. Mofokeng, K. De Wael, K. I. Ozoemena, *Omega*, **2022**, 7, 47892-47905. 74

3 132) O. O. Fashedemi, K. I. Ozoemena, *Sensors and Actuators B: Chemical*, **2011**, 160, 7-14. 76

4 133) A. Barhoum, R. J. Forster, *Anal Chim Acta*, **2022**, 12257, 340226. 78

5 134) N. S. Mathebula, J. Pillay, G. Toschi, J. A. Verschoor, K. Ozoemena, *Chem Commun (Camb)*, **2009**, 3345-3347. 80

6 135) J. Pillay, K. I. Ozoemena, R. T. Tshikhudo, R. Moutloali, *Langmuir*, **2010**, 26. 82

7 136) K. I. Ozoemena, N. S. Mathebula, J. Pillay, G. Toschi, J. Verschoor, *Phys Chem Chem Phys*, **2010**, 12, 345-357. 84

8 137) T. Bertok, L. Lorencova, E. Chocholova, E. Jane, Vikartovska, P. Kasak, J. Tkac, *ChemElectroChem*, **2018**, 6, 989-1003. 87

9 138) T. B. Tran, S. J. Son, J. Min, *BioChip J.*, **2016**, 10, 318-338. 88

10 139) E. B. Bahadir, M. K. Sezginurk, *Artif Cells Nanomed Biotechnol*, **2016**, 44, 248-262. 90

11 140) P. Aspermaier, V. Mishyn, J. Binting, H. Happy, K. Bages, P. Subramanian, W. Knoll, R. Boukherroub, S. Szunerit, *Anal Bioanal Chem*, **2021**, 413, 779-787. 93

12 141) B. M. Wormald, N. Moser, N. M. de Souza, K. Mantikas, K. Malpartida-Cardenas, I. Pennisi, T. E. J. Ince, K. Vroobel, M. Kalofonou, J. Rodriguez-Manzano, Georgiou, *Sci Rep*, **2022**, 12, 8750. 97

13 142) N. Gao, T. Gao, X. Yang, X. Dai, W. Zhou, A. Zhang, C. Lieber, *Proc Natl Acad Sci U S A* 2016, 113, 14633-14638. 98

14 143) N. Lu, A. Gao, P. Dai, S. Song, C. Fan, Y. Wang, T. Li, *Sensors*, **2014**, 10, 2022-2028. 101

15 144) K. I. Chen, B. R. Li, Y. T. Chen, *Nano Today*, **2011**, 6, 131-154. 103

16 145) H. B. Halima, A. Errachid, N. Jaffrezic-Renault, *Electroanalysis* **2021**, 35. 105

17 146) P. G. Gopinath, V. R. Anitha, Aruna Mastani, *Alexandria Engineering Journal*, **2018**, 57, 671-681. 107

18 147) F. Keyvani, N. Debnath, M. Ayman Saleh, M. Poudineh, *Nanoscale*, **2022**, 14, 6761-6770. 109

19 148) M. Bartosik, H. Durikova, B. Vojtesek, M. Anton, Jandakova, R. Hrstka, *Biosens Bioelectron*, **2016**, 83, 300-305. 112

20 149) S. Jampasa, W. Wonsawat, N. Rodthongkum, Siangproh, P. Yanatatsaneejit, T. Vilaivan, Chailapakul, *Biosens Bioelectron*, **2014**, 54, 428-434. 115

21 150) J.R. Espinosa, M. Galvan, A.S. Quinones, J.L. Ayala, Avila, S.M. Duron, *Molecules*, **2021**, 26, 3436. 117

22 151) C. X. Du, L. H., S. L. Dong, L. H. Li, Y. Wei, *Materials Science and Engineering*, **2016**, 137. 119

23 152) N. B. Mincu, V. Lazar, D. Stan, C.M. Mihailescu, R. Los, A.L. Mateescu, *Diagnostics (Basel)*, **2020**, 10. 121

24 153) J.R. Espinosa, M. Galvan, A.S. Quinones, J.L. Ayala, Avila, S.M. Duron, *Molecules*, **2021**, 26, 3436. 123

25 154) S. Cinti, V. Mazzaracchio, I. Cacciotti, D. Moscone, Arduini, *Sensors*, **2017**, 17, 2267. 124

26 155) J.P. Metters, S.M. Houssein, D.K. Kampouris, C.E. Barakat, *Anal. Methods* **2013**, 5, 103-110. 127

27 156) E. Noviana, C.P. McCord, K.M. Clark, I. Jang, C.S. Hedrick, *Lab Chip*, **2020**, 20, 9-34. 129

28 157) J. Zhang, Z. Yang, Q. Liu, H. Liang, *Talanta*, **2019**, 200, 384-391. 131

29 158) F. Arduini, S. Cinti, V. Caratelli, L. Amendola, G. Palleschi, D. Moscone, *Biosens Bioelectron*, **2019**, 126, 346-354. 133

30 159) Y. Wang, J. Luo, J. Liu, S. Sun, Y. Xiong, Y. Ma, S. Yan, Yang, H. Yin, X. Cai, *Biosens Bioelectron*, **2019**, 136, 835-90. 136

31 160) H. Wang, J. Wang, G. Liu, Z. Zhang, X. Hou, *Int J Electrochem. Sci.*, **2019**, 14, 11253-11266. 136

32 161) S. Cinti, C. Minotti, D. Moscone, G. Palleschi, F. Arduini, *Biosens Bioelectron*, **2017**, 93, 46-51. 136

33 162) A. Sánchez-Calvo, M.T. Fernández-Abedul, M.C. Blanco-López, A. Costa-García, *Sensors and Actuators B: Chemical*, **2019**, 290, 87-92. 136

34 163) M.L. Scala-Benuzzi, J. Raba, G. Soler-Illia, R.J. Schneider, G.A. Messina, *Anal Chem*, **2018**, 90, 4104-4111. 136

35 164) D. Jemmeli, E. Marcoccio, D. Moscone, C. Dridi, F. Arduini, *Talanta* **2020**, 216, 120924. 136

36 165) G.V. Martins, A.C. Marques, E. Fortunato, M.G.F. Sales, *Electrochimica Acta*, **2018**, 284, 60-68. 136

37 166) M.R. Tomei, S. Cinti, N. Interino, V. Manovella, D. Moscone, F. Arduini, *Sensors and Actuators B: Chemical*, **2019**, 294, 291-297. 136

38 167) M. Amatongchai, J. Sitanurak, W. Sroysee, S. Sodanath, S. Chairam, P. Jarujamrus, D. Nacapricha, P. Lieberzeit, *Anal Chim Acta*, **2019**, 1077, 255-265. 136

39 168) E. Solhi, M. Hasanzadeh, P. Babaie, *Analytical Methods* **2020**, 12, 1398-1414. 136

40 169) W. Dungchai, O. Chailapakul, C.S. Henry, A low-cost, simple, and rapid fabrication method for paper-based microfluidics using wax screen-printing. *Analyst*, **2011**, 136, 77-82. 136

41 170) Y. Sameenoi, P.N. Nongkai, S. Nouanthavong, C.S. Henry, D. Nacapricha, *Analyst*, **2014**, 139, 6580-6588. 136

42 171) A. Yakoh, S. Chaiyo, W. Siangproh, O. Chailapakul, *ACS Sens* 2019, 4, 1211-1221. 136

43 172) M.S. Draz, M. Moazeni, M. Venkataramani, H. Lakshminarayanan, E. Saygili, N.K. Lakshminarasimulu, K.M. Kochehyoki, M.K. Kanakasabapathy, S. Shabahang, A. Vasani, M. A. Bijarchi, A. Memic, H. Shafiee, *Adv Funct Mater* 2018, 28, 1707161 136

44 173) M. C. C. G. Carneiro, L.R. Rodrigues, F.T.C. Moreira, M.G.F. Sales, *Sensors (Basel)* 2022, 22, 3221. 136

45 174) T. Akyazi, L. Basabe-Desmonts, F. Benito-Lopez, *Anal Chim Acta* **2018**, 1001, 1-17. 136

46 175) S. Naorungroj, P. Teengam, T. Vilaivan, O. Chailapakul, *New Journal of Chemistry*, **2021**, 45, 6960-6967. 136

47 176) B. Hunt, A. Ruiz, B. Pogue, *J Biomed Opt*, **2021**, 26, 040902. 136

48 177) D. Erickson, D. O'Dell, L. Jiang, V. Oncescu, A. Gumus, S. Lee, M. Mancuso, S. Mehta, *Lab Chip*, **2014**, 14, 3159-3164. 136

49 178) C. Gallay, A. Girardet, M. Viviano, R. Catarino, A.C. Benski, P.L. Tran, C. Ecabert, J.P. Thiran, P. Vassilakos, P. Petignat, *Int J Womens Health*, **2017**, 9, 455-461. 136

50 179) C. Mungo, C.O. Osongo, J. Ambaka, M.A. Randa, M. B. Samba, C.A. Ochieng, E. Barker, A. Guliam, J. Omoto, C.R. Cohen, *JCO Glob Oncol*, **2021**, 7, 686-693. 136

51 180) D. Champin, M.C. Ramirez-Soto, J. Vargas-Herrera, *Cancers (Basel)*, **2021**, 13, 6047. 136

52 181) E. Dufeil, B. Kenfack, E. Tincho, J. Fouogue, A. Wisniak, J. Sormani, P. Vassilakos, P. Petignat, *PLoS One*, **2022**, 17. 136

53 182) A.H. Rossmann, H.W. Reid, M.M. Pieters, C. Mizelle, M. von Isenburg, N. Ramanujam, M.J. Huchko, L. Vasudevan, *J Med Internet Res*, **2021**, 23. 136

54 183) J. Sami, S. Lemoupa Makajio, E. Jeannot, B. Kenfack, R. Vinals, P. Vassilakos, P. Petignat, *Healthcare (Basel)*, **2022**, 10, 391. 136

55 184) Z. Dong, R. Hu, Y. Du, L. Tan, L. Li, J. Du, L. Bai, Y. Ma, H. Cui, *Front Immunol* **2020**, 11, 586796. 136

56 185) J. Makower, A. M., L. Denend, **2010**. 136

57 186) R. Hu, Z. Dong, K. Zhang, G. Pan, C. Li, H. Cui, *Viruses*, **2020**, 12, 333. 136

58 187) N. Manring, M.M.N. Ahmed, N. Tenhoff, J.L. Smeltz, P. Pathirathna, *Anal Chem*, **2022**, 94, 7149-7157. 136

Analytical Methods Accepted Manuscript

## Journal Name

## ARTICLE

- 188) Y. Jin, S.C. Kim, H.J. Kim, W. Ju, Y.H. Kim, *Glycobiology*, **2016**, 26, 100-107.
- 189) B. Hayes, C. Murphy, A. Crawley, R. O'Kennedy, *Diagnostics (Basel)*, **2018**, 8, 39.
- 190) R. Hernandez-Lopez, L. Hermsillo, L. Leon-Maldonado, R. Velazquez-Cruz, L. Torres-Ibarra, E. Lazcano-Ponce, A. Lorincz, C.M. Wheeler, F.X. Bosch, J. Cuzick, B. Rivera-Paredes, B. Nedjai, J. Salmeron, *PLoS One*, **2021**, 16.
- 191) Y. Chen, J. Wei, S. Zhang, H. Dai, L. Lv, Y. Lin, *J. Chem. Eng.*, **2022**, 436.
- 192) D. Pathania, C. Landeros, L. Rohrer, V. D'Agostino, S. Hong, I. Degani, M. Avila-Wallace, M. Pivovarov, T. Randall, R. Weissleder, et al., *Theranostics*, **2019**, 9, 8438-8447.

View Article Online  
DOI: 10.1039/D4AY01921K

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Open Access Article. Published on 23 December 2024. Downloaded on 16/2025 3:11:52 PM.  
This article is licensed under a Creative Commons Attribution 3.0 Unported Licence.





**Data availability**

View Article Online  
DOI: 10.1039/D4AY01921K

No primary research results, software or code have been included and no new data were generated or analysed as part of this review.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Open Access Article. Published on 23 December 2024. Downloaded on 16/12/2024 11:52 PM.  
This article is licensed under a Creative Commons Attribution 3.0 Unported Licence.

